

产品分析证书
Certificate of Analysis

中文名称: 表告依春

English Name: Epigoitrin

别名 (Alias):

产品编码 (Cat. No.): BP0543


CAS Number: 1072-93-1

分子式 (M. F.): C₅H₇NOS

分子量 (M. W.): 129.177

批号 (Batch No.): PRF8060721

报告日期 (Report date): 2017-06-07

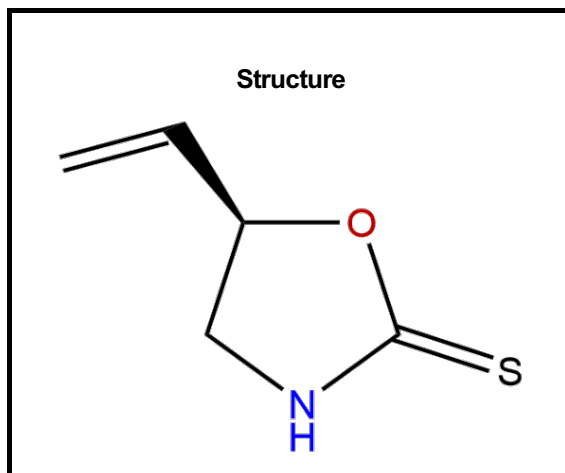

检验结果 (Analytical result):

检验项目 (Test Item)	检验指标 (Specifications)	检验结果 (Results)
外观 Appearance	Off-white powder	Off-white powder
干燥失重 Loss on drying	<3.0%	1.04%
纯度 Purity (HPLC-DAD, 240nm)*	≥98.0%	99.22%
质谱 Mass	129.1±1	Conforms
核磁 NMR	Comply with the structure	Conforms

* 色谱图见附件 (Please find HPLC chromatography attached.)

检测方法 (Test Method): Column: Thermo Hypersil GOLD AQ C18, 4.6*250mm, 5.0um; Column temperature: 30°C; Detection Mode: UV240nm; Flow

Rate: 1.0ml/min; Sample dissolution: 50% Methanol in water; Mobile Phase: A Triethylamine- Phosphoric acid in Water (PH=7) B, Acetonitrile; Gradient elution: B, 5%-10%, 15min.

贮存条件 (Storage): 2~8°C, protected from light, keep package airproofed when not in use.

复测期 (Retest date): two years (2019-06-06) under conditions list above.

QC: Zhang Ling

Date: 2017-06-07

QA: Wu Qi

Date: 2017-06-07

备注 (Remarks): The sample solutions should be prepared and used on the day of receipt. It is the best preparing the solutions immediately before use. If the solutions have to be made up in advance, it should be made as aliquots in tightly sealed vials at less than -20°C. Generally, these might be useable for up to two weeks.
In case of quality issue, please contact us within 15 days after receipt of the product.


Tel: +86-28-82633397 Fax: +86-28-82633165

http://www.phytopurify.com Email: sales@biopurify.com biopurify@gmail.com

SAMPLE INFORMATION

Sample Name:	Epigoitrin PRF8060721	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	
Vial:	2	Acq. Method Set:	Epigoitrin
Injection #:	1	Processing Method:	Samples
Injection Volume:	5.00 ul	Channel Name:	240.0nm
Run Time:	20.0 Minutes	Proc. Chnl. Descr.:	PDA 240.0 nm
Date Acquired:	2017-6-7 10:53:50 CST		
Date Processed:	2017-6-7 12:44:24 CST		

Auto-Scaled Chromatogram

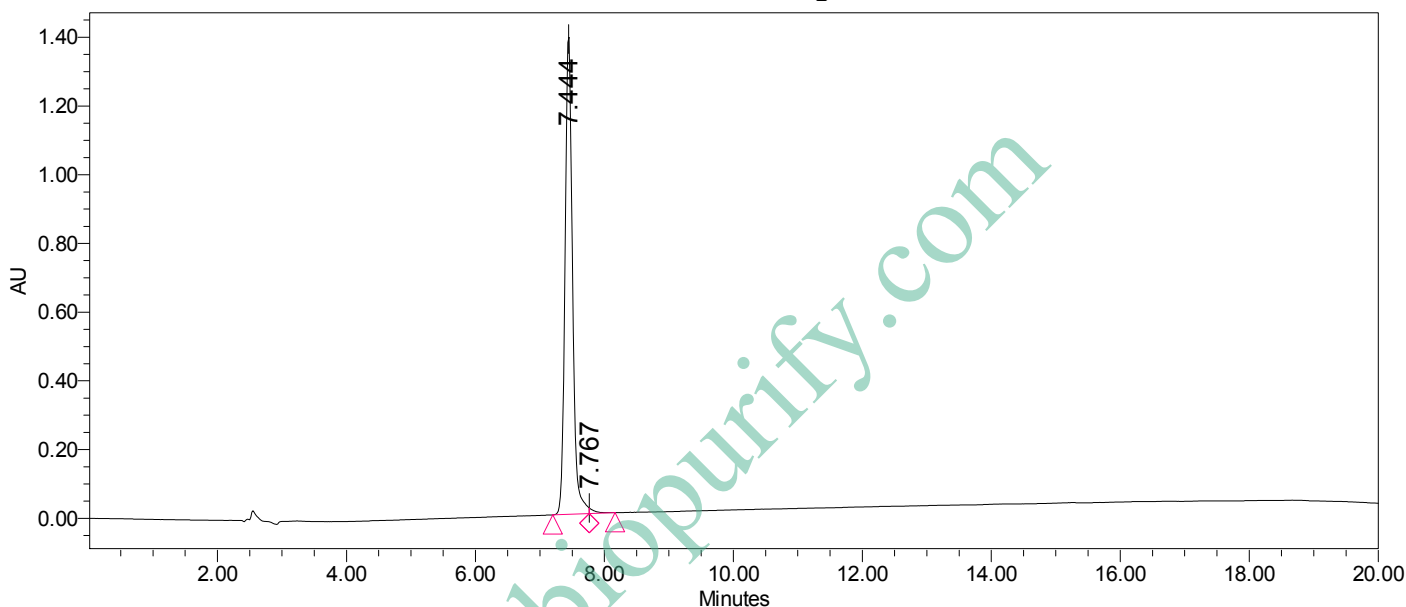


Peak Results

	Name	RT	Area	% Area	USP Plate Count	USP Resolution
1		7.444	11177784	99.22	21674.5	
2		7.767	87921	0.78		1.5

SAMPLE INFORMATION

Sample Name:	Epigoitrin Blank	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	
Vial:	40	Acq. Method Set:	Epigoitrin
Injection #:	1	Processing Method:	Samples
Injection Volume:	5.00 ul	Channel Name:	240.0nm
Run Time:	20.0 Minutes	Proc. Chnl. Descr.:	PDA 240.0 nm
Date Acquired:	2017-6-7 11:22:15 CST		
Date Processed:	2017-6-7 11:59:14 CST		

Auto-Scaled Chromatogram

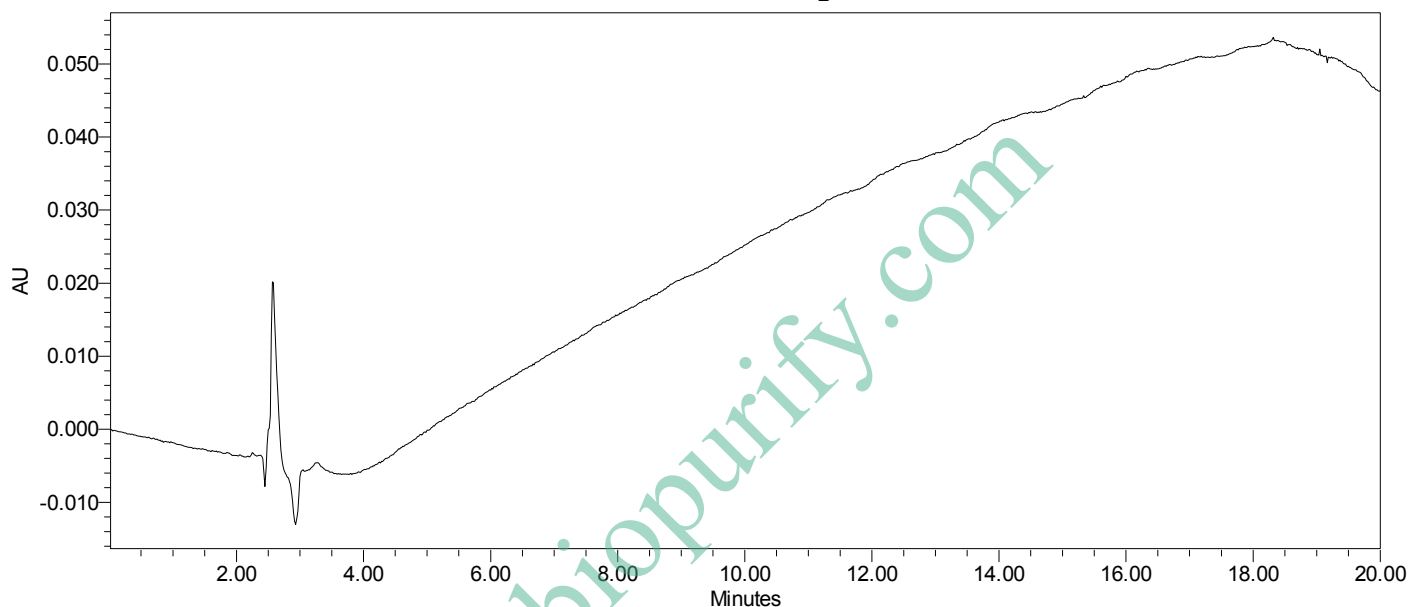

Peak Results

	Name	RT	Area	% Area	USP Plate Count	USP Resolution
1						