

产品分析证书
Certificate of Analysis

中文名称: 土贝母苷丙

English Name: Tubeimoside III

别名 (Alias):

产品编码 (Cat. No.): BP1482


CAS Number: 115810-13-4

分子式 (M. F.): C₆₄H₁₀₀O₃₁

分子量 (M. W.): 1365.47

批号 (Batch No.): PRF8070702

报告日期 (Report date): 2017-07-11

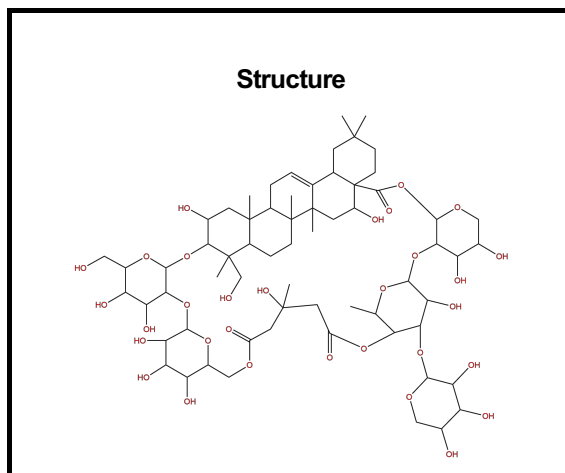

检验结果 (Analytical result):

检验项目 (Test Item)	检验指标 (Specifications)	检验结果 (Results)
外观 Appearance	Off-white powder	Off-white powder
纯度 Purity (HPLC-DAD, 205nm)*	≥98.0%	98.53%
质谱 Mass	1365.4±1	Conforms
核磁 NMR	Comply with the structure	Conforms
水分 Water Content	<3.0%	2.7%

* 色谱图见附件 (Please find HPLC chromatography attached.)

检测方法 (Test Method): Column: Thermo HYPURITY C18, 4.6*150mm, 3.0um; Column temperature: 30°C; Detection Mode: UV205nm;

Flow Rate: 1.0ml/min; Sample dissolution: Methanol; Mobile Phase: A, 0.1% phosphoric acid in water B, Acetonitrile; Gradient elution: B, 25%-35%, 20min.

贮存条件 (Storage): 2~8°C, protected from light, keep package airtight when not in use.

复测期 (Retest date): two years (2019-07-10) under conditions list above.

QC: Zhang Ling

Date: 2017-07-11

QA: Wu Qi

Date: 2017-07-11

备注 (Remarks): The sample solutions should be prepared and used on the same day. It is the best preparing the solutions immediately before use. If the solutions have to be made up in advance, it should be made as aliquots in tightly sealed vials at less than -20°C. Generally, these might be useable for up to two weeks.

In case of quality issue, please contact us within 15 days after receipt of the product.


Tel: +86-28-82633397 Fax: +86-28-82633165

http://www.phytopurify.com Email: sales@biopurify.com biopurify@gmail.com

SAMPLE INFORMATION

Sample Name:	Tubeimoside III PRF8070702	Acquired By:	System
Sample Type:	Standard	Sample Set Name:	
Vial:	32	Acq. Method Set:	Tubeimoside III
Injection #:	1	Processing Method:	Samples
Injection Volume:	10.00 ul	Channel Name:	205.0nm
Run Time:	25.0 Minutes	Proc. Chnl. Descr.:	PDA 205.0 nm
Date Acquired:	2017-7-11 9:20:31 CST		
Date Processed:	2017-7-11 10:42:54 CST		

Auto-Scaled Chromatogram

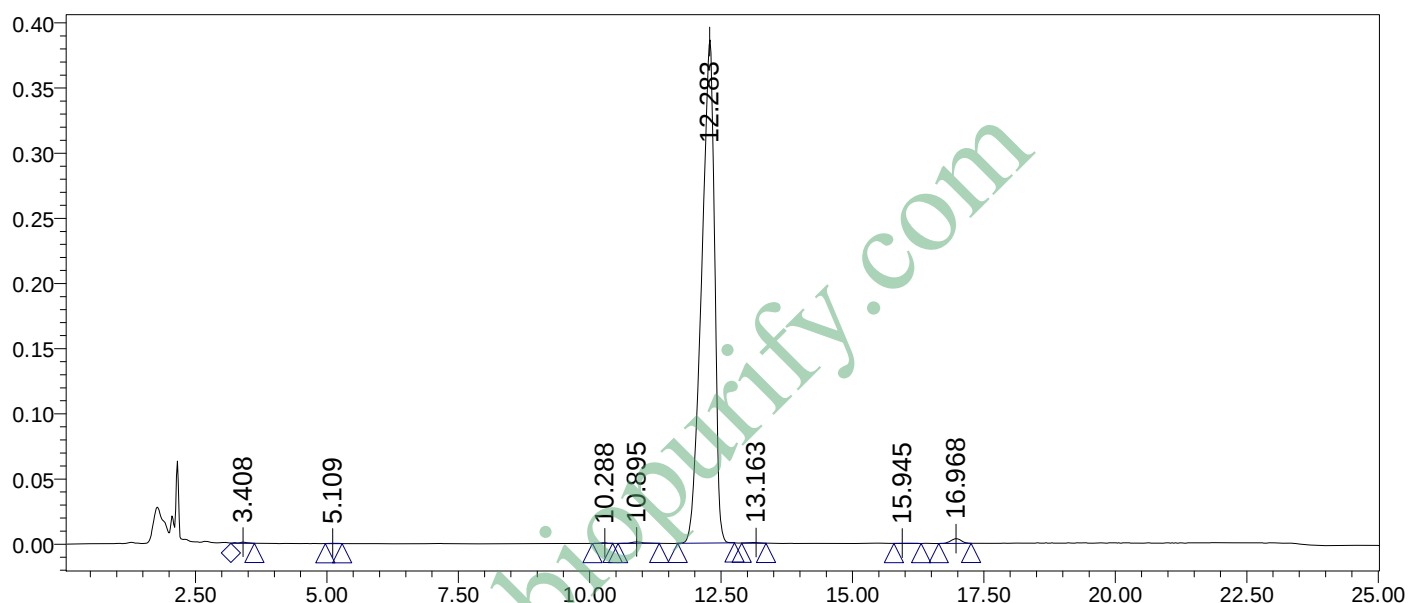

Peak Results

	RT	Area	% Area	USP Plate Count	USP Resolution
1	3.408	10703	0.16	3950.61	
2	5.109	3453	0.05	9549.36	3.04
3	10.288	5484	0.08	21280.87	20.13
4	10.895	16341	0.24	16308.82	1.84
5	12.283	6610228	98.53	9810.27	3.25
6	13.163	8325	0.12	14780.97	1.87
7	15.945	5057	0.08	38914.43	5.32
8	16.968	49482	0.74	35943.83	2.11