

产品分析证书
Certificate of Analysis

中文名称：茯苓新酸A

English Name : Poricoic acid A

别名(Alias): Poricoic acid F

产品编码(Cat. No.):BP1838


CAS Number: 137551-38-3

分子式(M. F.): C₃₁H₄₆O₅

分子量(M. W.): 498.704

批号(Batch No.): PRF8081143

报告日期(Report date): 2017-08-11

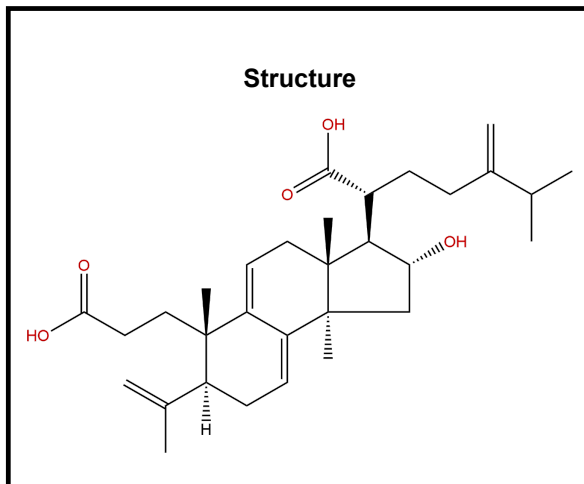

检验结果 (Analytical result) :

检验项目 (Test Item)	检验指标 (Specifications)	检验结果 (Results)
外观Appearance	Off-white cotton-like solid	Off-white cotton-like solid
干燥失重Loss on drying	< 3.0%	1.2%
纯度Purity (HPLC-DAD,240nm)*	≥97.0%	97.28%
质谱Mass	498.7±1	Conforms
核磁NMR	Comply with the structure	Conforms

* 色谱图见附件 (Please find HPLC chromatography attached.)

检测方法 (Test Method) : Column: Thermo HyPURITY C18 , 4.6*150mm , 3.0um; Column temperature: 30°C; Detection Mode:

UV240nm;Flow Rate: 1.0ml/min; Sample dissolution: Methanol; Mobile Phase: A, 0.1% phosphoric acid in water B, Acetonitrile;Gradient elution: B, 55%-70%,15min.

贮存条件 (Storage) :2~8°C, protected from light, keep package airproofed when not in use.

复测期 (Retest date) :two years (2019-08-10) under conditions list above.

QC: Zhang Ling

Date: 2017-08-11

QA: Wu Qi

Date: 2017-08-11

备注(Remarks): The sample solutions should be prepared on the same day, it is the best preparing the solutions immediately before use. If the solutions have to be made up in advance, it should be made as aliquots in tightly sealed vials at less than -20°C. Generally, these might be useable for up to two weeks.

In case of quality issue, please contact us within 15 days after receipt of the product.


Tel: +86-28-82633397 Fax: +86-28-82633165

http://www.phytopurify.com Email: sales@biopurify.com biopurify@gmail.com

SAMPLE INFORMATION

Sample Name:	Poricoic acid A PRF8081143	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	
Vial:	78	Acq. Method Set:	Poricoic acid A
Injection #:	1	Processing Method:	Samples
Injection Volume:	10.00 ul	Channel Name:	240.0nm
Run Time:	25.0 Minutes	Proc. Chnl. Descr.:	PDA 240.0 nm
Date Acquired:	2017-8-11 13:54:10 CST		
Date Processed:	2017-8-11 14:26:37 CST		

Auto-Scaled Chromatogram

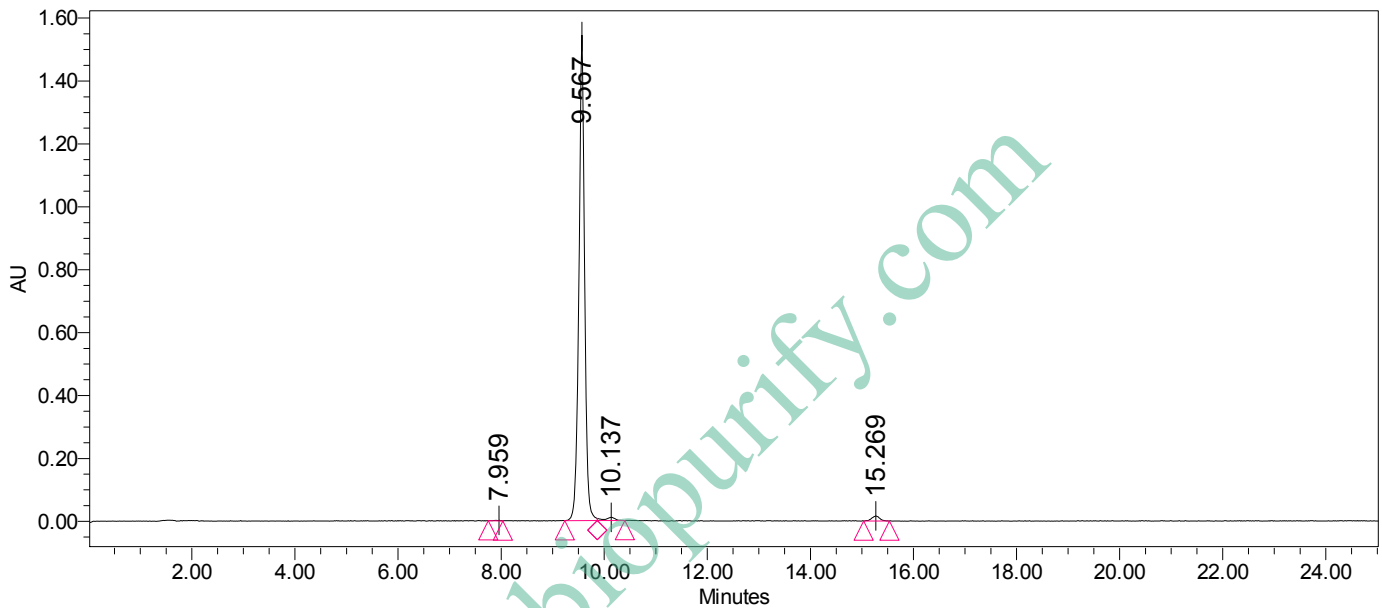

Peak Results

	Name	RT	Area	% Area	USP Plate Count	USP Resolution
1		7.959	13815	0.11	28700.4	
2		9.567	11985985	97.28	34320.7	7.2
3		10.137	153558	1.25		2.7
4		15.269	167582	1.36	42701.7	20.2