

产品分析证书 Certificate of Analysis

中文名称: 沙苑子苷A

English Name: Complanatoside A

别名 (Alias): Myricetin 3,4'-diglucoside

产品编码 (Cat. No.): BP0384


CAS Number: 146501-37-3

分子式 (M. F.): C₂₇H₃₀O₁₈

分子量 (M. W.): 642.519

批号 (Batch No.): PRF8031425

报告日期 (Report date): 2017年3月14日

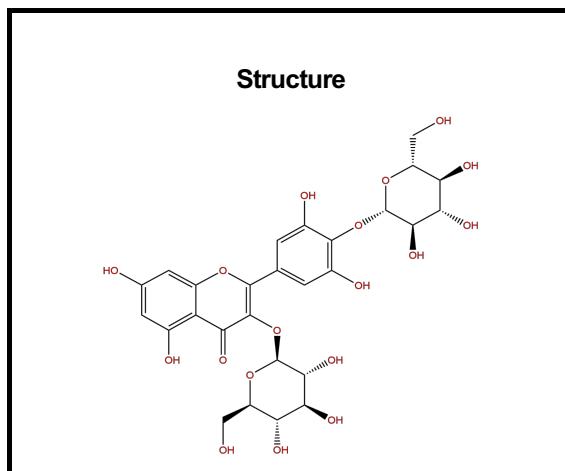

检验结果 (Analytical result):

检验项目 (Test Item)	检验指标 (Specifications)	检验结果 (Results)
外观 Appearance	Light yellow powder	Light yellow powder
干燥失重 Loss on drying	<3.0%	1.32%
纯度 Purity (HPLC-DAD, 267nm)*	≥95.0%	96.09%
质谱 Mass	642.519±1	Conforms
核磁 NMR	Comply with the structure	Conforms

* 色谱图见附件 (Please find HPLC chromatography attached.)

检测方法 (Test Method): Column: Thermo Hypersil GOLD AQ C18, 4.6*250mm, 5.0um; Column temperature: 30°C; Detection Mode: UV267nm; Flow

Rate: 1.0ml/min; Sample dissolution: 50% DMF in methanol; Mobile Phase: A, 0.1% Phosphate acid in water; B, Acetonitrile; Gradient elution:

B, 15%-35%, 15min.

贮存条件 (Storage): 2~8°C, protected from light, keep package airtight when not in use.

复测期 (Retest date): two years (2019-03-13) under conditions list above.

QC: Zhang Ling

Date: 2017年3月14日

QA: Wu Qi

Date: 2017年3月14日

备注 (Remarks): The sample solutions should be prepared and used immediately. It is the best preparing the solutions immediately before use. If the solutions have to be made up in advance, it should be made as aliquots in tightly sealed vials at less than -20°C. Generally, these might be useable for up to two weeks.

In case of quality issue, please contact us within 15 days after receipt of the product.


Tel: +86-28-82633397 Fax: +86-28-82633165

http://www.phytopurify.com Email: sales@biopurify.com biopurify@gmail.com

SAMPLE INFORMATION

Sample Name:	Complanatoside A PRF8031425	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	
Vial:	26	Acq. Method Set:	Complanatoside A
Injection #:	1	Processing Method:	Samples
Injection Volume:	10.00 ul	Channel Name:	267.0nm
Run Time:	22.0 Minutes	Proc. Chnl. Descr.:	PDA 267.0 nm
Date Acquired:	2017-3-14 14:28:48 CST		
Date Processed:	2017-3-14 15:02:23 CST		

Auto-Scaled Chromatogram

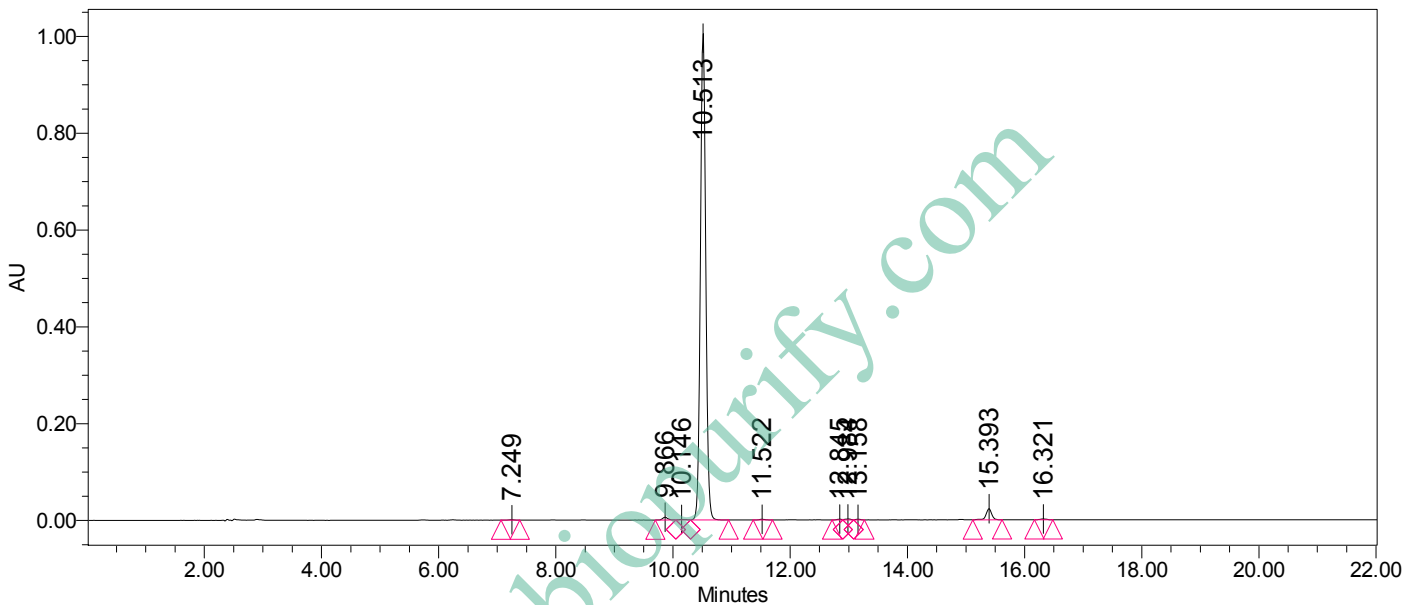

Peak Results

	Name	RT	Area	% Area	USP Plate Count	USP Resolution
1		7.249	7440	0.11	21729.7	
2		9.866	37950	0.58	54514.3	14.6
3		10.146	10176	0.15	16133.4	1.6
4		10.513	6338183	96.09	64373.9	2.1
5		11.522	9711	0.15	53022.3	5.4
6		12.845	7386	0.11	79980.1	6.5
7		12.984	11933	0.18	70365.3	0.7
8		13.158	6498	0.10	118011.5	1.0
9		15.393	153522	2.33	130680.3	13.4
10		16.321	13548	0.21	97292.0	4.9