

产品分析证书
Certificate of Analysis

中文名称: 杨梅苷

English Name: Myricetrin

别名 (Alias): Myricitroside; Myricetin 3- rhamnoside

产品编码 (Cat. No.): BP0971


CAS Number: 17912-87-7

分子式 (M. F.): C₂₁H₂₀O₁₂

分子量 (M. W.): 464.379

批号 (Batch No.): PRF8031443

报告日期 (Report date): 2017年3月14日

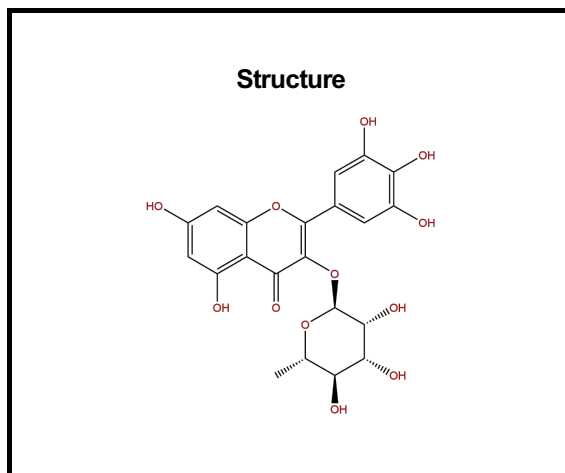

检验结果 (Analytical result):

检验项目 (Test Item)	检验指标 (Specifications)	检验结果 (Results)
外观 Appearance	Off-white powder	Off-white powder
干燥失重 Loss on drying	<3.0%	1.11%
纯度 Purity (HPLC-DAD, 263nm)*	≥98.0%	98.63%
质谱 Mass	464.379±1	Conforms
核磁 NMR	Comply with the structure	Conforms

* 色谱图见附件 (Please find HPLC chromatography attached.)

检测方法 (Test Method): Column: Thermo Hypersil GOLD AQ C18, 4.6*250mm, 5.0um; Column temperature: 30°C; Detection Mode: UV263nm; Flow

Rate: 1.0ml/min; Sample dissolution: 20% methanol in water; Mobile Phase: A, 0.1% Phosphate acid in water B, Acetonitrile; Gradient elution: B, 10%-30%, 15min.

贮存条件 (Storage): 2~8°C, protected from light, keep package airtight when not in use.

复测期 (Retest date): two years (2019-03-13) under conditions list above.

QC: Zhang Ling

Date: 2017年3月14日

QA: Wu Qi

Date: 2017年3月14日

备注 (Remarks): The sample solutions should be prepared and used immediately. It is the best preparing the solutions immediately before use. If the solutions have to be made up in advance, it should be made as aliquots in tightly sealed vials at less than -20°C. Generally, these might be useable for up to two weeks.

In case of quality issue, please contact us within 15 days after receipt of the product.


Tel: +86-28-82633397 Fax: +86-28-82633165

http://www.phytopurify.com Email: sales@biopurify.com biopurify@gmail.com

SAMPLE INFORMATION

Sample Name:	Myricetrin PRF8031443	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	
Vial:	55	Acq. Method Set:	Myricetrin
Injection #:	1	Processing Method:	Samples
Injection Volume:	10.00 ul	Channel Name:	263.0nm
Run Time:	22.0 Minutes	Proc. Chnl. Descr.:	PDA 263.0 nm
Date Acquired:	2017-3-14 15:02:32 CST		
Date Processed:	2017-3-14 15:36:03 CST		

Auto-Scaled Chromatogram

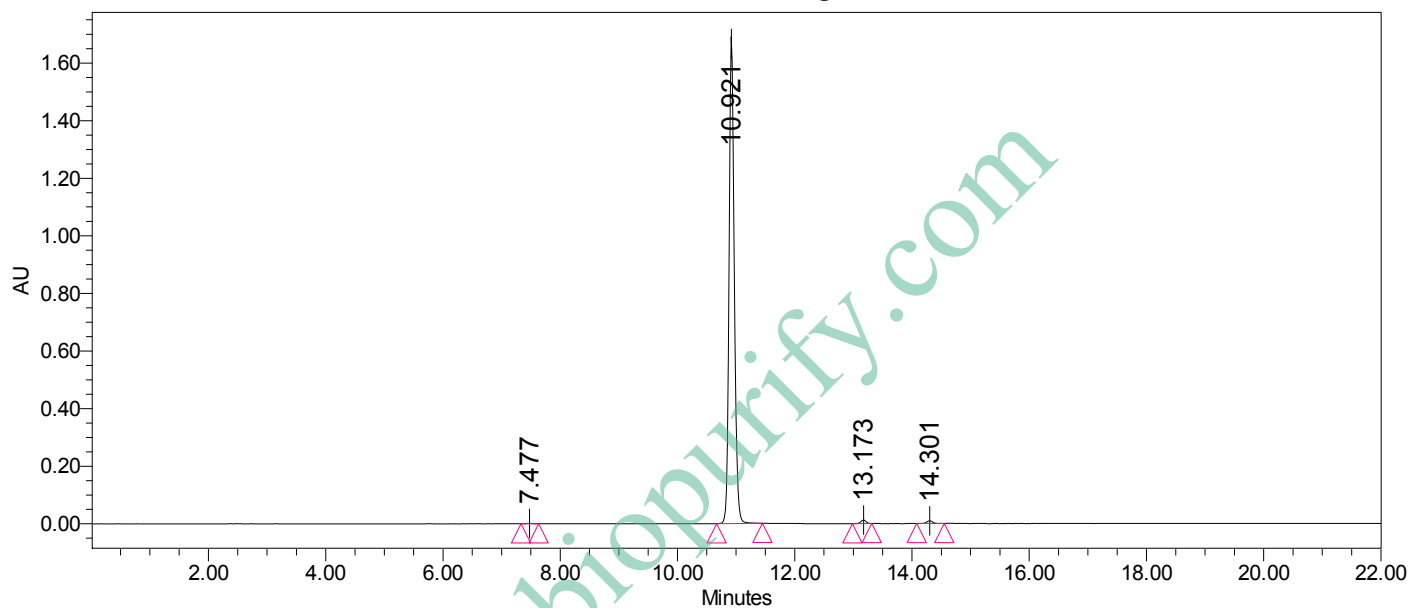

Peak Results

	Name	RT	Area	% Area	USP Plate Count	USP Resolution
1		7.477	6896	0.06	26601.3	
2		10.921	10557726	98.63	70519.6	19.5
3		13.173	74213	0.69	107280.7	13.4
4		14.301	65762	0.61	106810.3	6.5