

产品分析证书 Certificate of Analysis

中文名称: 1,5-二咖啡酰奎宁酸

English Name: 1,5-Dicaffeoylquinic acid

别名 (Alias):

产品编码 (Cat. No.): BP0006


CAS Number: 19870-46-3

分子式 (M. F.): C₂₅H₂₄O₁₂

分子量 (M. W.): 516.455

批号 (Batch No.): PRF8042142

报告日期 (Report date): 2017-04-21

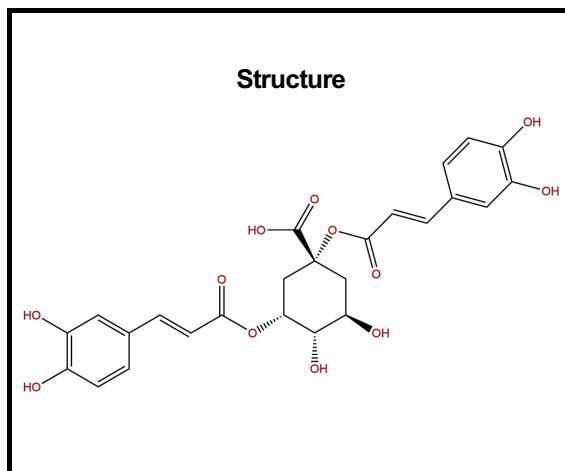

检验结果 (Analytical result):

检验项目 (Test Item)	检验指标 (Specifications)	检验结果 (Results)
外观 Appearance	Light yellow solid	Light yellow solid
干燥失重 Loss on drying	<3.0%	1.22%
纯度 Purity (HPLC-DAD, 330nm)*	≥98.0%	98.91%
质谱 Mass	516.4±1	Conforms
核磁 NMR	Comply with the structure	Conforms

* 色谱图见附件 (Please find HPLC chromatography attached.)

检测方法 (Test Method): Column: Agilent 5TC-C18, 4.6*150mm; Column temperature: 30°C; Detection Mode: UV330nm; Flow Rate:

1.0ml/min; Sample dissolution: 50% Acetonitrile in water; Mobile Phase: A, 0.1% Phosphoric acid in water B, Acetonitrile; Gradient elution: B,

15%-25%, 15min.

贮存条件 (Storage): 2~8°C, protected from light, keep package airproofed when not in use.

复测期 (Retest date): two years (2019-04-20) under conditions list above.

QC: Zhang Ling

Date: 2017-04-21

QA: Wu Qi

Date: 2017-04-21

备注 (Remarks): The sample solutions should be prepared and used immediately. It is the best preparing the solutions immediately before use. If the solutions have to be made up in advance, it should be made as aliquots in tightly sealed vials at less than -20°C. Generally, these might be useable for up to two weeks.

In case of quality issue, please contact us within 15 days after receiving the product.


Tel: +86-28-82633397 Fax: +86-28-82633165

http://www.phytopurify.com Email: sales@biopurify.com biopurify@gmail.com

SAMPLE INFORMATION

Sample Name:	1 5 Dicafeoylquinic acid	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	
Vial:	79	Acq. Method Set:	1 5 Dicafeoylquinic acid
Injection #:	1	Processing Method:	Samples
Injection Volume:	5.00 ul	Channel Name:	330.0nm
Run Time:	25.0 Minutes	Proc. Chnl. Descr.:	PDA 330.0 nm
Date Acquired:	2017-4-21 10:35:46 CST		
Date Processed:	2017-4-21 11:08:46 CST		

Auto-Scaled Chromatogram

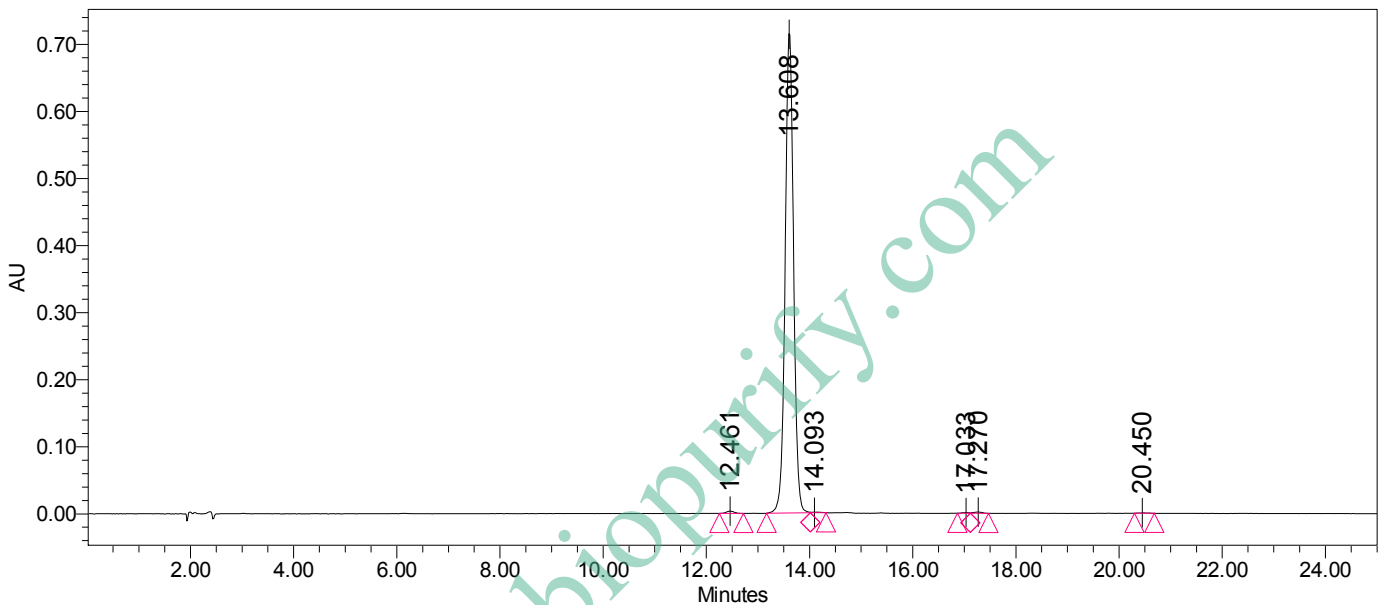

Peak Results

	Name	RT	Area	% Area	USP Plate Count	USP Resolution
1		12.461	37354	0.46	30577.4	
2		13.608	8062605	98.91	34620.4	4.0
3		14.093	14059	0.17		1.6
4		17.033	8102	0.10		
5		17.270	21856	0.27	32928.8	
6		20.450	7119	0.09	52164.1	7.7