

产品分析证书
Certificate of Analysis

中文名称: 京尼平苷

English Name: Geniposide

别名 (Alias): Genipin 1-glucoside; Jasminoidin

产品编码 (Cat. No.): BP0632


CAS Number: 24512-63-8

分子式 (M. F.): C₁₇H₂₄O₁₀

分子量 (M. W.): 388.369

批号 (Batch No.): PRF8030342

报告日期 (Report date): 2017年3月3日

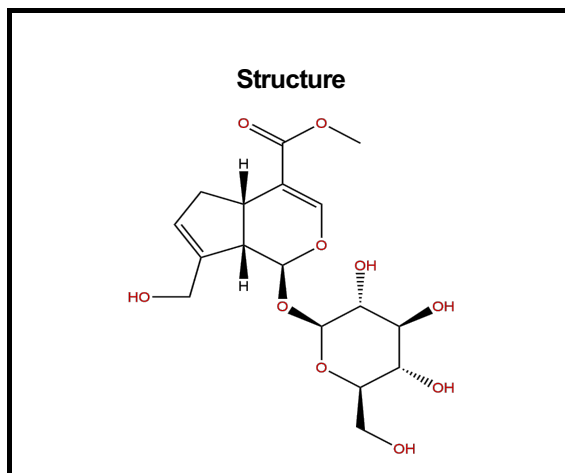

检验结果 (Analytical result):

检验项目 (Test Item)	检验指标 (Specifications)	检验结果 (Results)
外观 Appearance	Off-white powder	Off-white powder
干燥失重 Loss on drying	<3.0%	0.88%
纯度 Purity (HPLC-DAD, 240nm)*	≥98.0%	99.07%
质谱 Mass	388.369±1	Conforms
核磁 NMR	Comply with the structure	Conforms

* 色谱图见附件 (Please find HPLC chromatography attached.)

检测方法 (Test method): Column: Thermo BDS Hypersil C18 2.4μm 100 x 4.6 mm; Column temperature: 30°C; Flow Rate: 1.0ml/min;

Detection Mode: UV240nm; Sample dissolution: Water; Mobile Phase: A, 0.1% Phosphoric acid in water B, Acetonitrile; Gradient elution: B, 10%-15%, 15min.

贮存条件 (Storage): 2~8°C, protected from light, keep package airproofed when not in use.

复测期 (Retest date): two years (2019-03-02) under conditions list above.

QC: Zhang Ling
Date: 2017年3月3日



QA: Wu Qi
Date: 2017年3月3日

备注 (Remarks): The sample solutions should be prepared and used on the same day, it is the best preparing the solutions immediately before use. If the solutions have to be made up in advance, it should be made as aliquots in tightly sealed vials at less than -20°C. Generally, these might be useable for up to two weeks.

In case of quality issue, please contact us within 15 days after receipt of the product.


Tel: +86-28-82633397 Fax: +86-28-82633165

http://www.phytopurify.com Email: sales@biopurify.com biopurify@gmail.com

SAMPLE INFORMATION

Sample Name:	Geniposide PRF8030342	Acquired By:	System
Sample Type:	Standard	Sample Set Name:	
Vial:	7	Acq. Method Set:	Geniposide
Injection #:	1	Processing Method:	Samples
Injection Volume:	5.00 ul	Channel Name:	240.0nm
Run Time:	25.0 Minutes	Proc. Chnl. Descr.:	PDA 240.0 nm
Date Acquired:	2017-3-3 14:03:42 CST		
Date Processed:	2017-3-3 14:40:46 CST		

Auto-Scaled Chromatogram

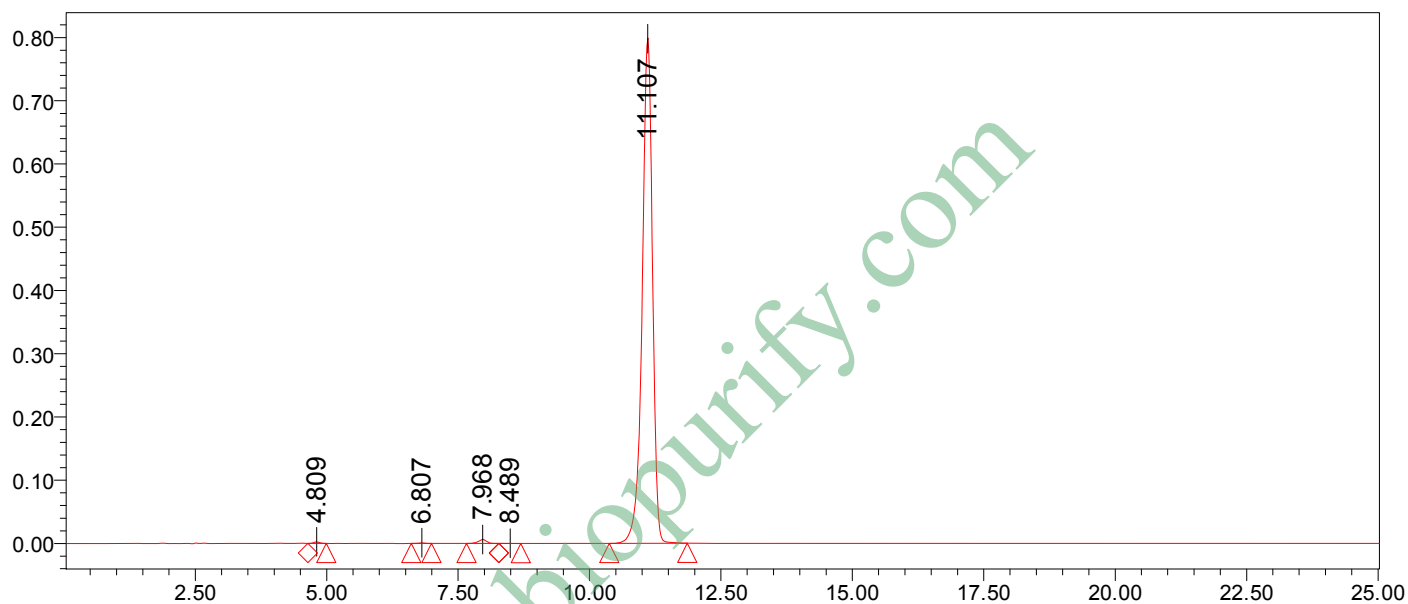

Peak Results

	RT	Area	% Area	USP Plate Count	USP Resolution
1	4.809	19521	0.18	8719.59	
2	6.807	8817	0.08	11296.75	8.61
3	7.968	67183	0.61	12238.04	4.22
4	8.489	6347	0.06	13303.90	1.75
5	11.107	10854417	99.07	16175.39	7.93