

产品分析证书 Certificate of Analysis

中文名称: 和蟾蜍他灵

English Name: Gamabufotalin

别名 (Alias): Gamabufagin; Gamabufogenin

产品编码 (Cat. No.): BP0612


CAS Number: 465-11-2

分子式 (M. F.): C₂₄H₃₄O₅

分子量 (M. W.): 402.531

批号 (Batch No.): PRF8060102

报告日期 (Report date): 2017-06-01

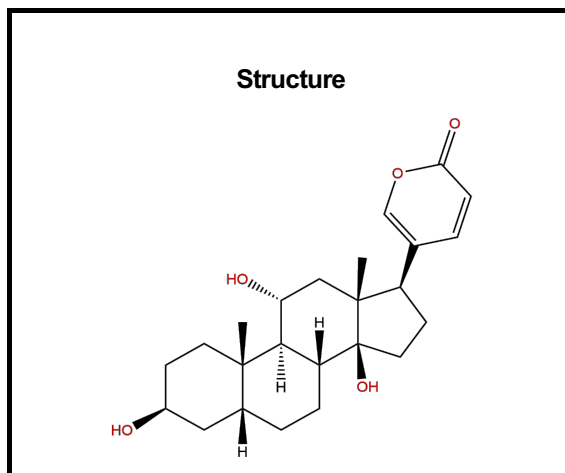

检验结果 (Analytical result):

检验项目 (Test Item)	检验指标 (Specifications)	检验结果 (Results)
外观 Appearance	Off-white powder	Off-white powder
纯度 Purity (HPLC-DAD, 300nm)*	≥98.0%	99.27%
质谱 Mass	402.5±1	Conforms
核磁 NMR	Comply with the structure	Conforms
水分 Water Content	<3.0%	0.87%

* 色谱图见附件 (Please find HPLC chromatography attached.)

检测方法 (Test Method): Column: Thermo Hypersil GOLD AQ C18, 4.6*250mm, 5.0um; Column temperature: 30°C; Detection Mode: UV300nm;

Flow Rate: 1.0ml/min; Sample dissolution: Methanol; Mobile Phase: A, 0.5% Potassium dihydrogen phosphate in water (Phosphoric acid adjusts PH to 3.2)

B, Acetonitrile; Isocratic elution: B, 20%.

贮存条件 (Storage): 2~8°C, protected from light, keep package airtight when not in use.

复测期 (Retest date): two years (2019-05-31) under conditions list above.

QC: Zhang Ling

Date: 2017-06-01

QA: Wu Qi

Date: 2017-06-01

备注 (Remarks): The sample solutions should be prepared and used on the day of analysis. It is the best preparing the solutions immediately before use. If the solutions have to be made up in advance, it should be made as aliquots in tightly sealed vials at less than -20°C. Generally, these might be useable for up to two weeks.
In case of quality issue, please contact us within 15 days after receipt of the product.


Tel: +86-28-82633397 Fax: +86-28-82633165

http://www.phytopurify.com Email: sales@biopurify.com biopurify@gmail.com

SAMPLE INFORMATION

Sample Name:	Gamabufotalin PRF8060102	Acquired By:	System
Sample Type:	Standard	Sample Set Name:	
Vial:	115	Acq. Method Set:	Gamabufotalin
Injection #:	5	Processing Method:	Samples
Injection Volume:	10.00 ul	Channel Name:	300.0nm
Run Time:	25.0 Minutes	Proc. Chnl. Descr.:	PDA 300.0 nm
Date Acquired:	2017-6-1 13:10:00 CST		
Date Processed:	2017-6-1 13:46:17 CST		

Auto-Scaled Chromatogram

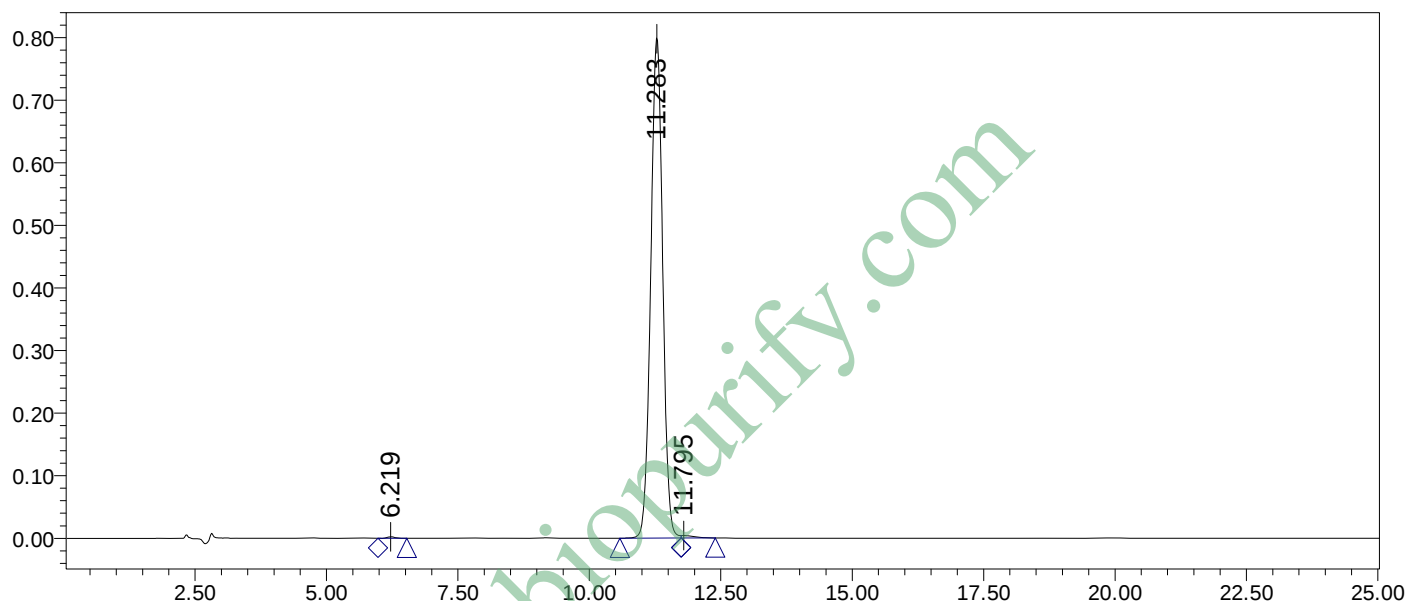

Peak Results

	RT	Area	% Area	USP Plate Count	USP Resolution
1	6.219	22140	0.17	10426.52	
2	11.283	12595984	99.27	11838.68	15.12
3	11.795	70343	0.55		