

产品分析证书
Certificate of Analysis

中文名称: 芥芬胺

English Name: Jervine

别名 (Alias): 17,23-Epoxy-3-hydroxyveratraman-11-one;
Jervin-11-one

产品编码 (Cat. No.): BP0810


CAS Number: 469-59-0

分子式 (M. F.): C₂₇H₃₉NO₃

分子量 (M. W.): 425.613

批号 (Batch No.): PRF8071443

报告日期 (Report date): 2017-07-17

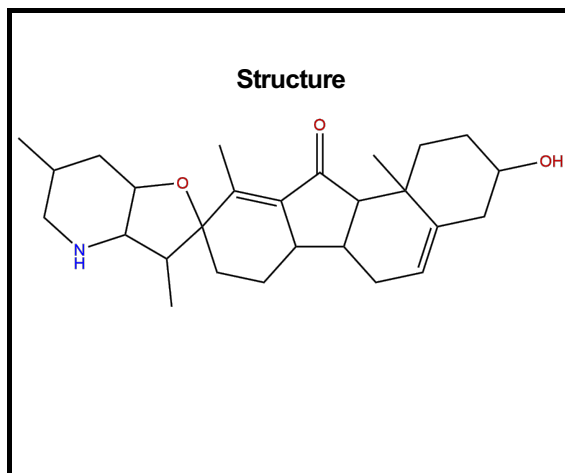

检验结果 (Analytical result):

检验项目 (Test Item)	检验指标 (Specifications)	检验结果 (Results)
外观 Appearance	Off-white cotton-like solid	Off-white cotton-like solid
干燥失重 Loss on drying	<3.0%	1.38%
纯度 Purity (HPLC-DAD, 251nm)*	≥98.0%	99.59%
质谱 Mass	425.6±1	Conforms
核磁 NMR	Comply with the structure	Conforms

* 色谱图见附件 (Please find HPLC chromatography attached.)

检测方法 (Test Method): Column: Thermo Hypersil GOLD AQ C18, 4.6*250mm, 5.0μm; Column temperature: 30°C; Detection Mode: UV251nm; Flow Rate: 1.0ml/min;

Sample dissolution: Methanol; Mobile Phase: A 0.1% TFA in water B, Acetonitrile; Gradient elution: B, 25%-35%, 15min.

贮存条件 (Storage): 2-8°C, protected from light, keep package airproofed when not in use.

复测期 (Retest date): two years (2019-07-16) under conditions list above.

QC: Zhang Ling

Date: 2017-07-17

QA: Wu Qi

Date: 2017-07-17

备注 (Remarks): The sample solutions should be prepared and used on the day of receipt. It is the best preparing the solutions immediately before use. If the solutions have to be made up in advance, it should be made as aliquots in tightly sealed vials at less than -20°C. Generally, these might be useable for up to two weeks.

In case of quality issue, please contact us within 15 days after receipt of the product.


Tel: +86-28-82633397 Fax: +86-28-82633165

http://www.phytopurify.com Email: sales@biopurify.com biopurify@gmail.com

SAMPLE INFORMATION

Sample Name:	Jervine PRF8071443	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	
Vial:	25	Acq. Method Set:	Jervine
Injection #:	1	Processing Method:	Samples
Injection Volume:	10.00 ul	Channel Name:	251.0nm
Run Time:	25.0 Minutes	Proc. Chnl. Descr.:	PDA 251.0 nm
Date Acquired:	2017-7-17 11:12:11 CST		
Date Processed:	2017-7-17 12:45:52 CST		

Auto-Scaled Chromatogram

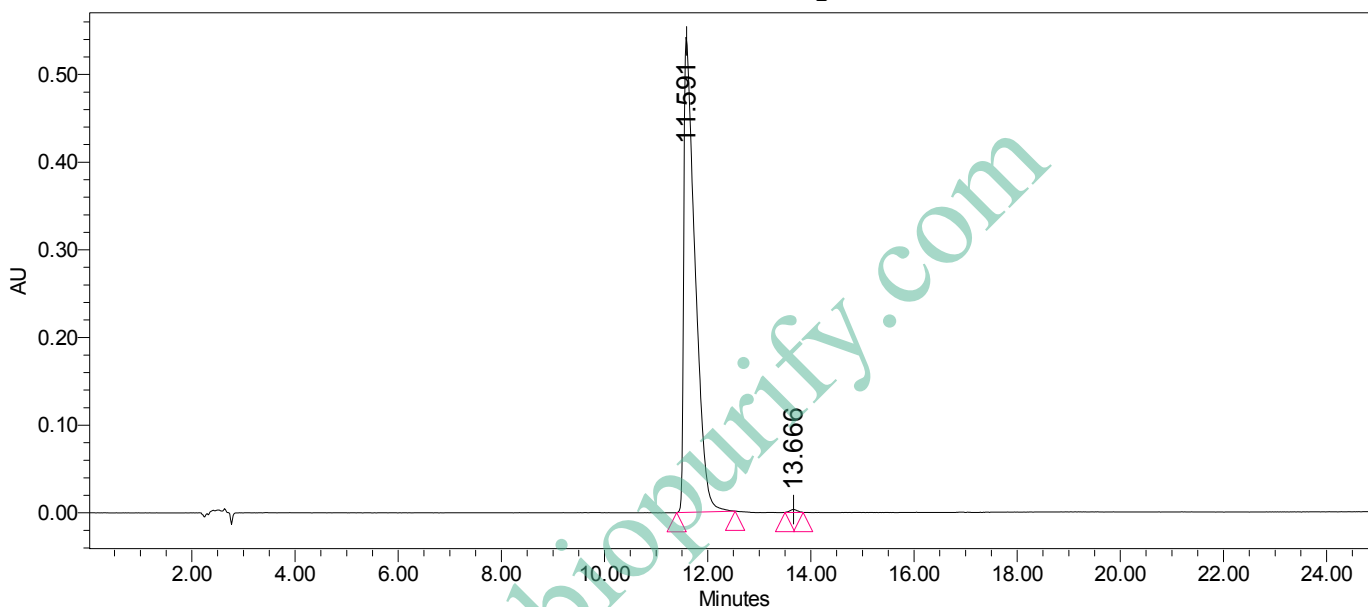

Peak Results

	Name	RT	Area	% Area	USP Plate Count	USP Resolution
1		11.591	8256635	99.59	11595.0	
2		13.666	34044	0.41	38122.5	5.7