

产品分析证书
Certificate of Analysis

中文名称: 瑞香素

English Name: Daphnetin

别名 (Alias): 7,8-Dihydroxycoumarin; Daphnetol

产品编码 (Cat. No.): BP0449


CAS Number: 486-35-1

分子式 (M. F.): C₉H₆O₄

分子量 (M. W.): 178.143

批号 (Batch No.): PRF8032822

报告日期 (Report date): 2017-03-28

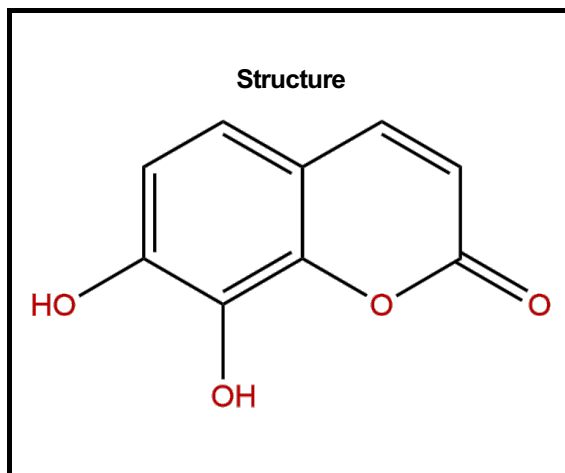

检验结果 (Analytical result):

检验项目 (Test Item)	检验指标 (Specifications)	检验结果 (Results)
外观 Appearance	Off-white cotton like solid	Off-white cotton like solid
干燥失重 Loss on drying	<3.0%	1.24%
纯度 Purity (HPLC-DAD, 324nm)*	≥98.0%	99.30%
质谱 Mass	178.143±1	Conforms
核磁 NMR	Comply with the structure	Conforms

* 色谱图见附件 (Please find HPLC chromatography attached.)

检测方法 (Test Method): Column: Agilent 5HC-C18, 4.6*250mm, 5.0um; Column temperature: 30°C; Detection Mode: UV324nm;

Flow Rate: 1.0ml/min; Sample dissolution: Methanol; Mobile Phase: A, 0.1% phosphoric acid in water B, Acetonitrile; Gradient elution: B, 15%-40%, 15min.

贮存条件 (Storage): 2~8°C, protected from light, keep package airproofed when not in use.

复测期 (Retest date): two years (2019-03-27) under conditions list above.

QC: Zhang Ling

Date: 2017-03-28

QA: Wu Qi

Date: 2017-03-28

备注 (Remarks): The sample solutions should be prepared and used on the same day. It is the best preparing the solutions immediately before use. If the solutions have to be made up in advance, it should be made as aliquots in tightly sealed vials at less than -20°C. Generally, these might be useable for up to two weeks.

In case of quality issue, please contact us within 15 days after receipt of the product.


Tel: +86-28-82633397 Fax: +86-28-82633165

http://www.phytopurify.com Email: sales@biopurify.com biopurify@gmail.com

SAMPLE INFORMATION

Sample Name:	Daphnetin	Acquired By:	System
Sample Type:	Standard	Sample Set Name:	
Vial:	35	Acq. Method Set:	Daphnetin
Injection #:	1	Processing Method:	Samples
Injection Volume:	5.00 ul	Channel Name:	324.0nm
Run Time:	25.0 Minutes	Proc. Chnl. Descr.:	PDA 324.0 nm
Date Acquired:	2017-3-28 11:44:10 CST		
Date Processed:	2017-3-28 12:36:01 CST		

Auto-Scaled Chromatogram

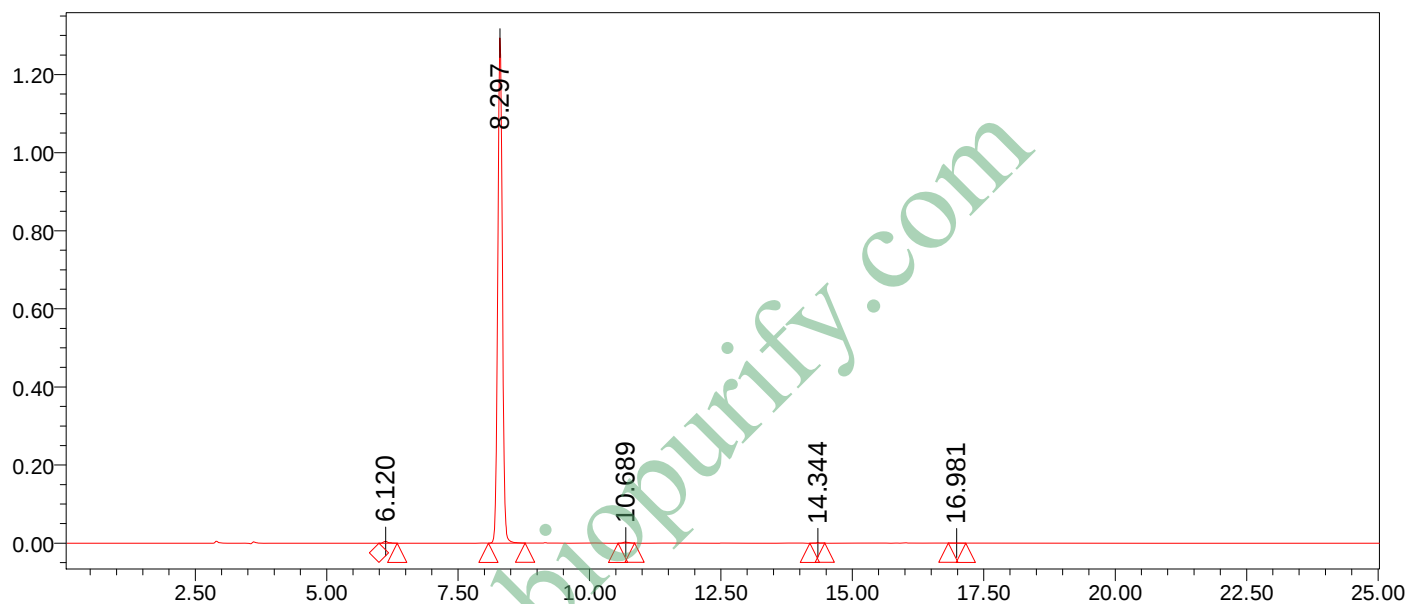

Peak Results

	RT	Area	% Area	USP Plate Count	USP Resolution
1	6.120	28814	0.36	24611.87	
2	8.297	7854343	99.30	42686.81	13.37
3	10.689	18416	0.23	56885.47	13.62
4	14.344	3867	0.05	107189.07	19.86
5	16.981	3962	0.05	96268.39	12.97