

产品分析证书
Certificate of Analysis

中文名称: 泽兰黄酮

English Name: Eupafolin

别名 (Alias): Nepetin; 6-Methoxyluteolin; 3',4',5,7-Tetrahydroxy-6-methoxyflavone

产品编码 (Cat. No.): BP1615


CAS Number: 520-11-6

分子式 (M. F.): C₁₆H₁₂O₇

分子量 (M. W.): 316.265

批号 (Batch No.): PRF8052222

报告日期 (Report date): 2017-05-22

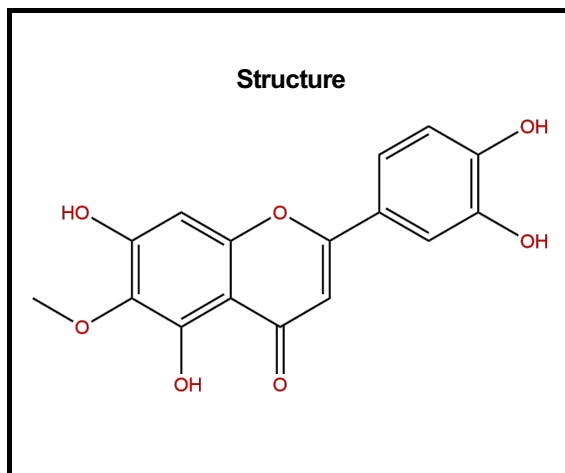

检验结果 (Analytical result):

检验项目 (Test Item)	检验指标 (Specifications)	检验结果 (Results)
外观 Appearance	Yellow powder	Yellow powder
干燥失重 Loss on drying	<3.0%	1.05%
纯度 Purity (HPLC-DAD, 345nm)*	≥98.0%	99.57%
质谱 Mass	316.2±1	Conforms
核磁 NMR	Comply with the structure	Conforms

* 色谱图见附件 (Please find HPLC chromatography attached.)

检测方法 (Test Method): Column: Thermo Hypersil GOLD AQ C18, 4.6*250mm, 5.0um; Column temperature: 30°C; Detection Mode: UV345nm; Flow

Rate: 1.0ml/min; Sample dissolution: Methanol; Mobile Phase: A, 0.1% Phosphoric acid in water B, Acetonitrile; Gradient elution: B, 25%-40%, 15min.

贮存条件 (Storage): -2~-8°C, protected from light, keep package airproofed when not in use.

复测期 (Retest date): two years (2019-05-21) under conditions list above.

QC: Zhang Ling
Date: 2017-05-22

QA: Wu Qi
Date: 2017-05-22

备注 (Remarks): The sample solutions should be prepared and used immediately. It is the best preparing the solutions immediately before use. If the solutions have to be made up in advance, it should be made as aliquots in tightly sealed vials at less than -20°C. Generally, these might be useable for up to two weeks.
In case of quality issue, please contact us within 15 days after receipt of the product.


Tel: +86-28-82633397 Fax: +86-28-82633165

http://www.phytopurify.com Email: sales@biopurify.com biopurify@gmail.com

SAMPLE INFORMATION

Sample Name:	Nepetin PRF8052222	Acquired By:	System
Sample Type:	Standard	Sample Set Name:	
Vial:	60	Acq. Method Set:	Nepetin
Injection #:	1	Processing Method:	Samples
Injection Volume:	10.00 ul	Channel Name:	345.0nm
Run Time:	25.0 Minutes	Proc. Chnl. Descr.:	PDA 345.0 nm
Date Acquired: 2017-5-22 11:20:08 CST			
Date Processed: 2017-5-22 12:54:25 CST			

Auto-Scaled Chromatogram

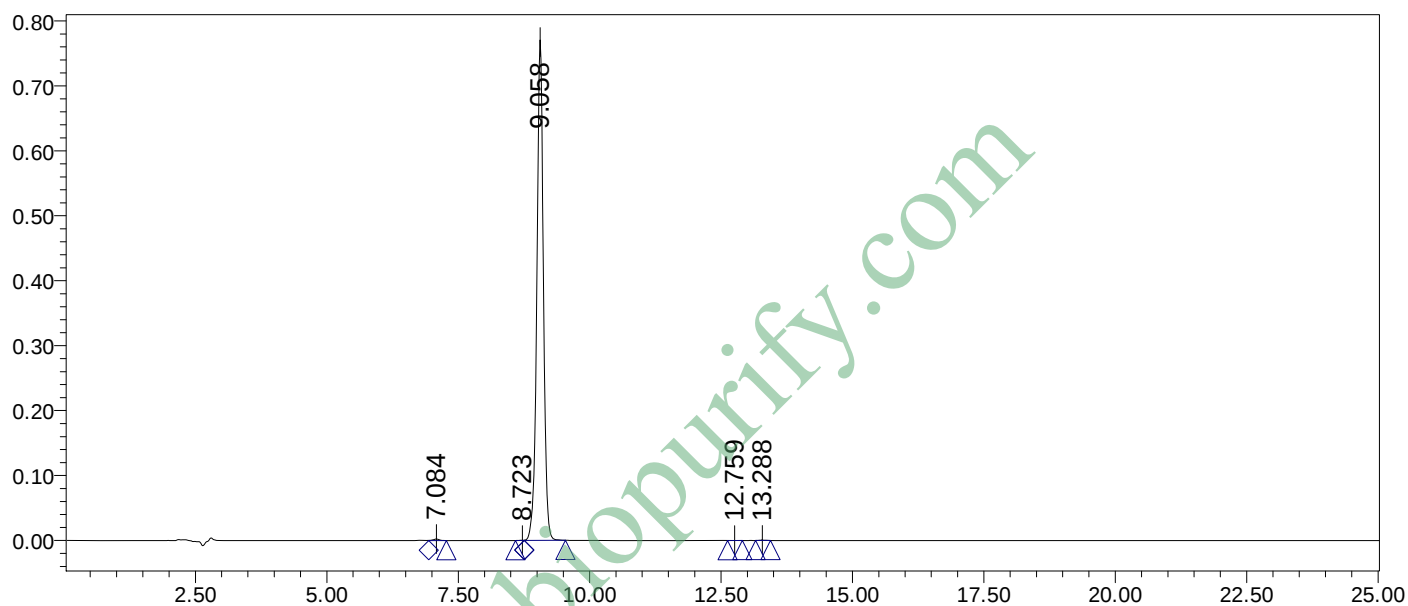

Peak Results

	RT	Area	% Area	USP Plate Count	USP Resolution
1	7.084	17328	0.26	19780.11	
2	8.723	2682	0.04		
3	9.058	6696688	99.57	26245.52	
4	12.759	4222	0.06	44049.14	15.85
5	13.288	4856	0.07	51038.20	2.28