



产品分析证书 Certificate of Analysis

中文名称: 高根二醇

English Name: OLEAN-12-ENE-3B,28-DIOL

别名 (Alias): 12-Ursen-3-beta,28-diol

产品编码 (Cat. No.): SBP01343


CAS Number: 545-46-0

分子式 (M. F.): C₃₀H₅₀O₂

分子量 (M. W.): 442.728

批号 (Batch No.): PRF8050527

报告日期 (Report date): 2017-05-05

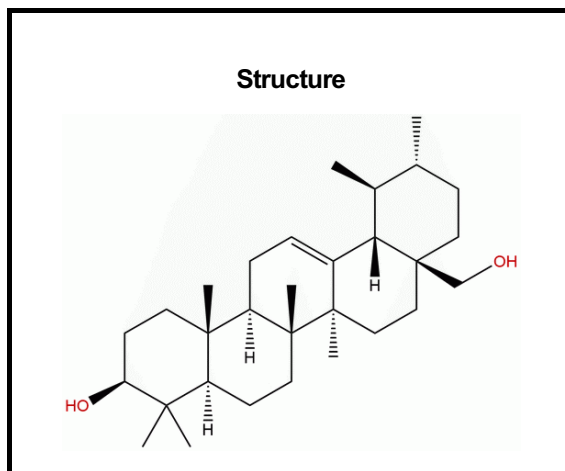

检验结果 (Analytical result):

检验项目 (Test Item)	检验指标 (Specifications)	检验结果 (Results)
外观 Appearance	Off-white powder	Off-white powder
干燥失重 Loss on drying	<3.0%	1.63%
纯度 Purity (HPLC-DAD, 205nm)*	≥98.0%	98.02%
质谱 Mass	442.7±1	Conforms
核磁 NMR	Comply with the structure	Conforms

* 色谱图见附件 (Please find HPLC chromatography attached.)

检测方法 (Test Method): Column: Thermo BDS Hypersil C18, 4.6*100mm, 2.4μm; Column temperature: 30°C; Detection Mode: UV274nm

Flow Rate: 1.0ml/min; Sample dissolution: Methanol; Mobile Phase: A, 0.1% Phosphoric acid in water B, Acetonitrile; Gradient elution: B, 75%-85%, 15min.

贮存条件 (Storage): 2~8°C, protected from light, keep package airtight when not in use.

复测期 (Retest date): two years (2019-05-04) under conditions list above.

QC: Zhang Ling

Date: 2017-05-05

QA: Wu Qi

Date: 2017-05-05

备注 (Remarks): The sample solutions should be prepared and used on the same day. It is the best preparing the solutions immediately before use. If the solutions have to be made up in advance, it should be made as aliquots in tightly sealed vials at less than -20°C. Generally, these might be useable for up to two weeks.

In case of quality issue, please contact us within 15 days after receipt of the product.




Tel: +86-28-82633397 Fax: +86-28-82633165

http://www.phytopurify.com Email: sales@biopurify.com biopurify@gmail.com

SAMPLE INFORMATION

Sample Name:	OLEAN 12 ENE 3B 28 DIOL	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	
Vial:	116	Acq. Method Set:	OLEAN 12 ENE 3B 28 DIOL
Injection #:	1	Processing Method:	Samples
Injection Volume:	10.00 ul	Channel Name:	205.0nm
Run Time:	25.0 Minutes	Proc. Chnl. Descr.:	PDA 205.0 nm
Date Acquired:	2017-5-5 15:05:25 CST		
Date Processed:	2017-5-5 15:36:51 CST		

Auto-Scaled Chromatogram

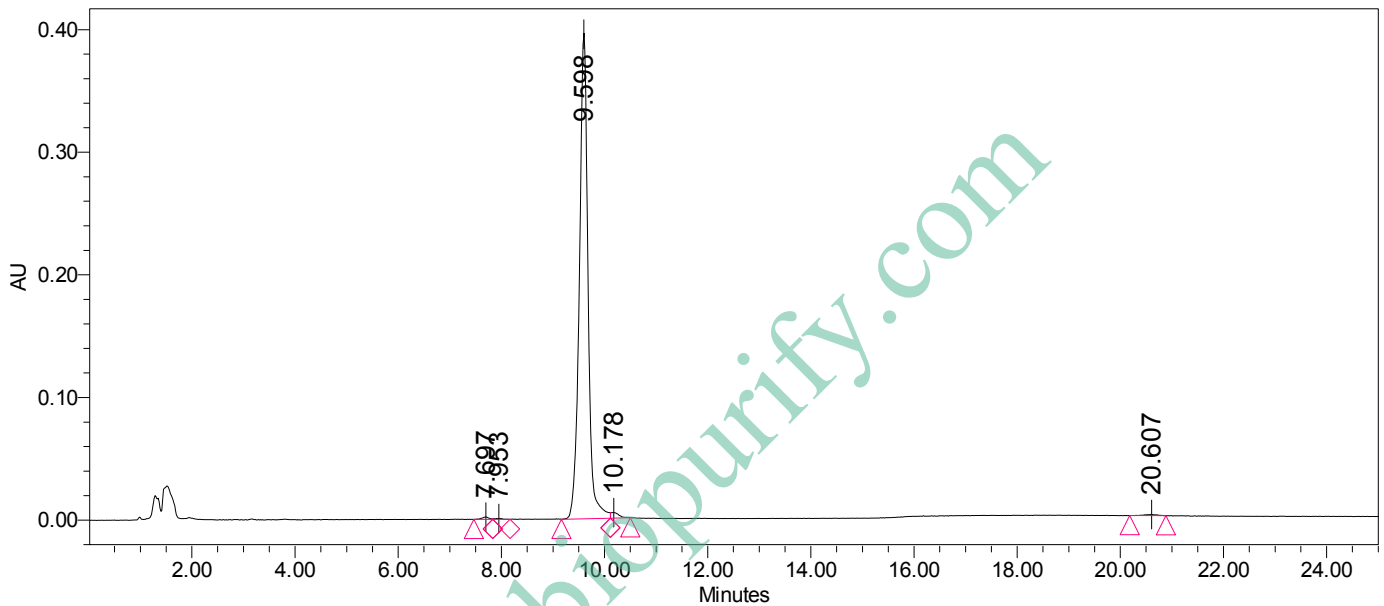

Peak Results

	Name	RT	Area	% Area	USP Plate Count	USP Resolution
1		7.697	19451	0.41	16994.0	
2		7.953	7950	0.17	8714.7	0.9
3		9.598	4606454	98.02	17395.1	6.0
4		10.178	49636	1.06		1.9
5		20.607	15795	0.34	30645.6	20.3