

产品分析证书 Certificate of Analysis

中文名称: 盐酸小檗胺

English Name: Berbamine dihydrochloride

别名 (Alias):

产品编码 (Cat. No.): BP0250


CAS Number: 6078-17-7

分子式 (M. F.): C₃₇H₄₁ClN₂O₆

分子量 (M. W.): 645.193

批号 (Batch No.): PRF8031042

报告日期 (Report date): 2017年3月10日

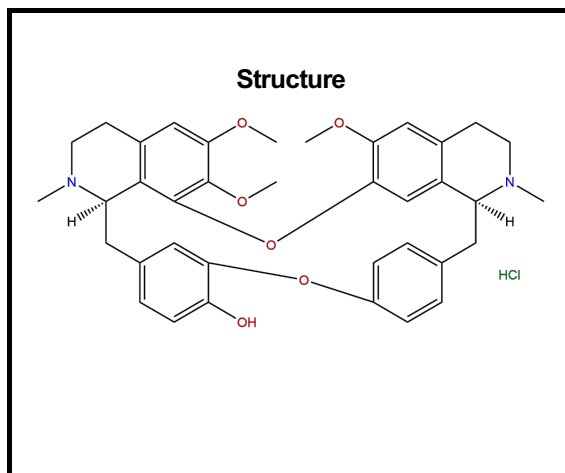

检验结果 (Analytical result):

检验项目 (Test Item)	检验指标 (Specifications)	检验结果 (Results)
外观 Appearance	Off-white powder	Off-white powder
干燥失重 Loss on drying	<3.0%	0.93%
纯度 Purity (HPLC-DAD, 282nm)*	≥98.0%	98.04%
质谱 Mass	645.193±1	Conforms
核磁 NMR	Comply with the structure	Conforms

* 色谱图见附件 (Please find HPLC chromatography attached.)

检测方法 (Test Method): Column: Thermo HYPURITY C18, 4.6*150mm, 3.0um; Column temperature: 30°C; Detection Mode: UV282nm;

Flow Rate: 1.0ml/min; Sample dissolution: Water; Mobile Phase: A, Triethylamine- Phosphate in Water (PH=2), B, Acetonitrile; Gradient elution: B, 20%-45%, 15min.

贮存条件 (Storage): 2~8°C, protected from light, keep package airtight when not in use.

复测期 (Retest date): two years (2019-03-09) under conditions list above.

QC: Zhang Ling

Date: 2017年3月10日

QA: Wu Qi

Date: 2017年3月10日

备注 (Remarks): The sample solutions should be prepared and used immediately. It is the best preparing the solutions immediately before use. If the solutions have to be made up in advance, it should be made as aliquots in tightly sealed vials at less than -20°C. Generally, these might be useable for up to two weeks.

In case of quality issue, please contact us within 15 days after receipt of the product.


Tel: +86-28-82633397 Fax: +86-28-82633165

http://www.phytopurify.com Email: sales@biopurify.com biopurify@gmail.com

SAMPLE INFORMATION

Sample Name:	Berbamine dihydrochloride	Acquired By:	System
Sample Type:	Standard	Sample Set Name:	
Vial:	5	Acq. Method Set:	Berbamine dihydrochloride
Injection #:	1	Processing Method:	Samples
Injection Volume:	15.00 ul	Channel Name:	282.0nm
Run Time:	25.0 Minutes	Proc. Chnl. Descr.:	PDA 282.0 nm
Date Acquired:	2017-3-10 15:14:39 CST		
Date Processed:	2017-3-10 16:11:30 CST		

Auto-Scaled Chromatogram

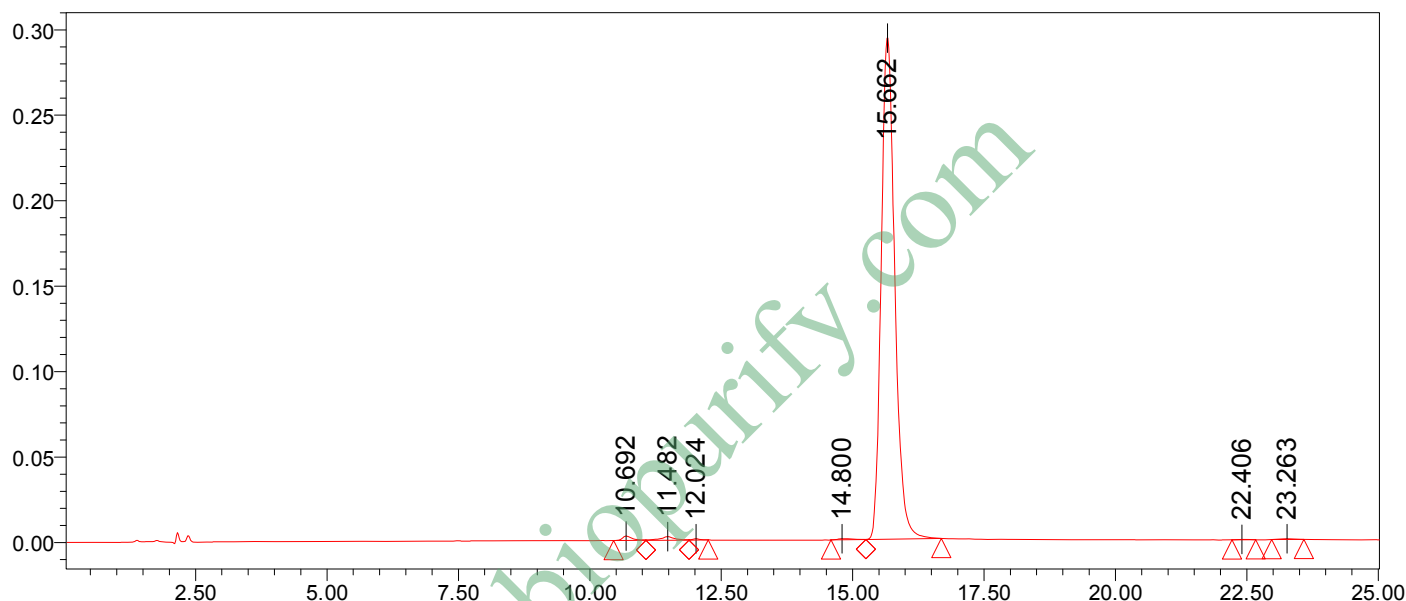

Peak Results

	RT	Area	% Area	USP Plate Count	USP Resolution
1	10.692	32632	0.61	18445.01	
2	11.482	38664	0.72	12895.84	1.90
3	12.024	7270	0.14	36854.63	1.42
4	14.800	12858	0.24	9300.38	6.86
5	15.662	5266855	98.04	17963.22	1.69
6	22.406	4877	0.09	61534.18	16.03
7	23.263	9220	0.17	24985.69	1.82