

产品分析证书
Certificate of Analysis

中文名称: 二水槲皮素

English Name: Quercetin Dihydrate

别名 (Alias): 3',4',5,7-Tetrahydroxyflavonol; Sophoretin;
Meletin; Quercetol; Quertin; Ericin

产品编码 (Cat. No.): BP1190


CAS Number: 6151-25-3

分子式 (M. F.): C₁₅H₁₀O₇

分子量 (M. W.): 302.238

批号 (Batch No.): PRF8070521

报告日期 (Report date): 2017-07-05

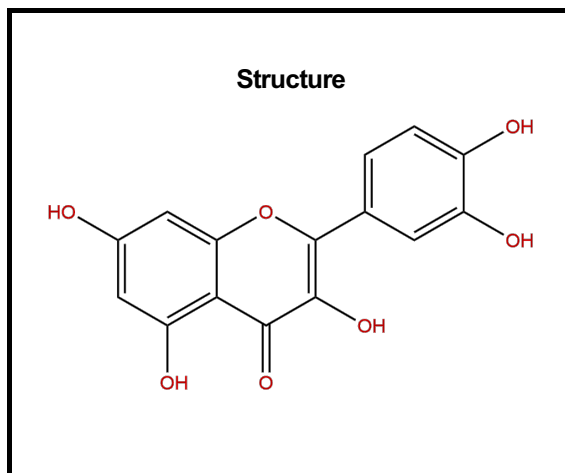

检验结果 (Analytical result):

检验项目 (Test Item)	检验指标 (Specifications)	检验结果 (Results)
外观 Appearance	Yellow-green powder	Yellow-green powder
纯度 Purity (HPLC-DAD, 370nm)*	≥95.0%	95.81%
质谱 Mass	302.2±1	Conforms
核磁 NMR	Comply with the structure	Conforms
水分 Water Content	<3.0%	1.87%

* 色谱图见附件 (Please find HPLC chromatography attached.)

检测方法 (Test Method): Column: Thermo Hypersil GOLD AQ C18, 4.6*250mm, 5.0um; Column temperature: 30°C; Detection Mode: UV370nm; Flow

Rate: 1.0ml/min; Sample dissolution: Methanol; Mobile Phase: A, 0.1% phosphoric acid in water B, Acetonitrile; Gradient elution: B, 25%-35%, 15min.

贮存条件 (Storage): -2~-8°C, protected from light, keep package airproofed when not in use.

复测期 (Retest date): two years (2019-07-04) under conditions list above.

QC: Zhang Ling

Date: 2017-07-05

QA: Wu Qi

Date: 2017-07-05

备注 (Remarks): The sample solutions should be prepared and used on the day of receipt. It is the best preparing the solutions immediately before use. If the solutions have to be made up in advance, it should be made as aliquots in tightly sealed vials at less than -20°C. Generally, these might be useable for up to two weeks.

In case of quality issue, please contact us within 15 days after receipt of the product.


Tel: +86-28-82633397 Fax: +86-28-82633165

http://www.phytopurify.com Email: sales@biopurify.com biopurify@gmail.com

SAMPLE INFORMATION

Sample Name:	Quercetin Dihydrate PRF8070521	Acquired By:	System
Sample Type:	Standard	Sample Set Name:	
Vial:	24	Acq. Method Set:	Quercetin Dihydrate
Injection #:	1	Processing Method:	Samples
Injection Volume:	10.00 ul	Channel Name:	370.0nm
Run Time:	25.0 Minutes	Proc. Chnl. Descr.:	PDA 370.0 nm
Date Acquired:	2017-7-5 9:43:42 CST		
Date Processed:	2017-7-5 10:22:29 CST		

Auto-Scaled Chromatogram

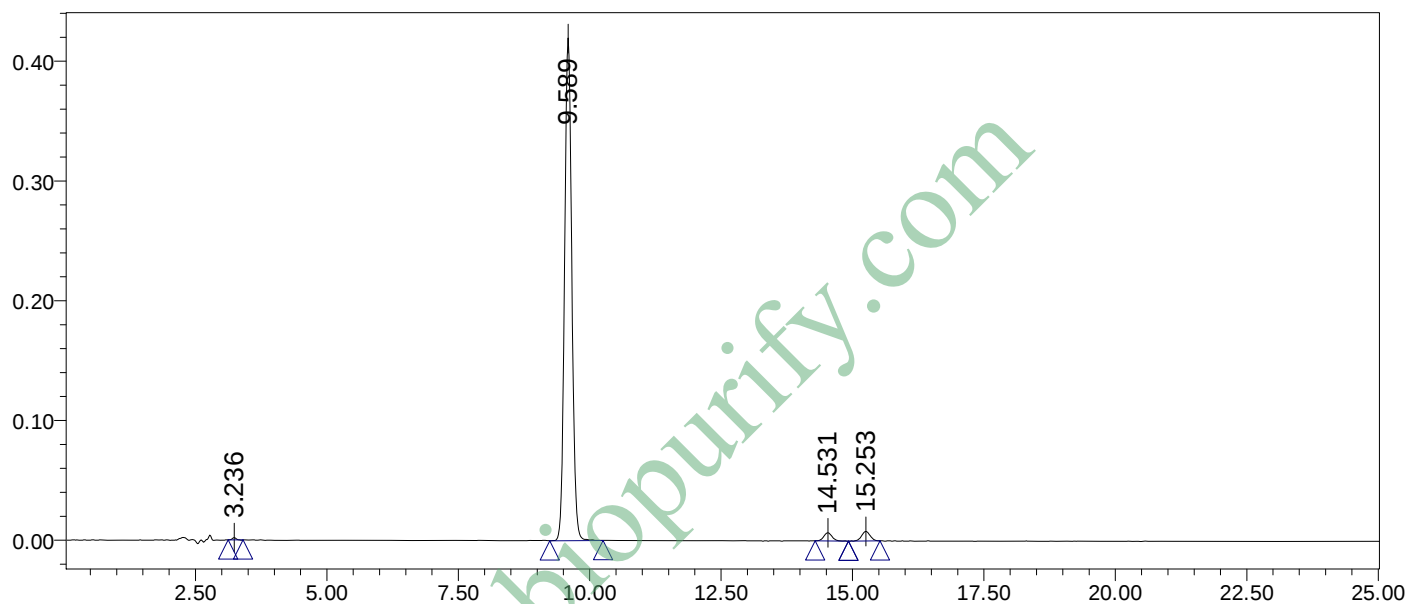

Peak Results

	RT	Area	% Area	USP Plate Count	USP Resolution
1	3.236	10124	0.24	8563.22	
2	9.589	4005881	95.81	23338.35	32.09
3	14.531	75554	1.81	37932.84	17.76
4	15.253	89572	2.14	41293.52	2.37