

产品分析证书
Certificate of Analysis

中文名称: 伪原纤细薯蓣皂苷

English Name: Pseudoprotogracillin

别名 (Alias):

产品编码 (Cat. No.): BP3334


CAS Number: 637349-03-2

分子式 (M. F.): C₅₁H₈₂O₂₂

分子量 (M. W.): 1047.2

批号 (Batch No.): PRF8071821

报告日期 (Report date): 2017-07-18

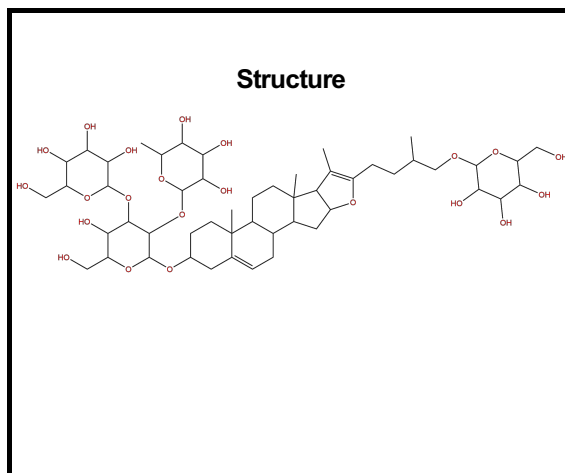

检验结果 (Analytical result):

检验项目 (Test Item)	检验指标 (Specifications)	检验结果 (Results)
外观 Appearance	Off-white solid	Off-white solid
干燥失重 Loss on drying	<3.0%	2.14%
纯度 Purity (HPLC-ELSD)*	≥96.0%	96.44%
质谱 Mass	1047.2±1	Conforms
核磁 NMR	Comply with the structure	Conforms

* 色谱图见附件 (Please find HPLC chromatography attached.)

检测方法 (Test Method): Column: Thermo BDS Hypersil C18, 4.6*100mm, 2.4μm; Column temperature: 30°C; Detection Mode: ELSD;

Flow Rate: 1.0ml/min; Sample dissolution: Methanol; Mobile Phase: A Water B, Acetonitrile; Gradient elution: B, 25%-40%, 15min.

贮存条件 (Storage): 2~8°C, protected from light, keep package airtight when not in use.

复测期 (Retest date): two years (2019-07-17) under conditions list above.

QC: Zhang Ling

Date: 2017-07-18

QA: Wu Qi

Date: 2017-07-18

备注 (Remarks): The sample solutions should be prepared and used on the same day. It is the best preparing the solutions immediately before use. If the solutions have to be made up in advance, it should be made as aliquots in tightly sealed vials at less than -20°C. Generally, these might be useable for up to two weeks.

In case of quality issue, please contact us within 15 days after receipt of the product.


Tel: +86-28-82633397 Fax: +86-28-82633165

http://www.phytopurify.com Email: sales@biopurify.com biopurify@gmail.com

SAMPLE INFORMATION

Sample Name:	Pseudoprotogracillin PRF8071821	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	
Vial:	23	Acq. Method Set:	Pseudoprotogracillin
Injection #:	1	Processing Method:	Samples
Injection Volume:	10.00 ul	Channel Name:	SATIN
Run Time:	25.0 Minutes	Proc. Chnl. Descr.:	
Date Acquired:	2017-7-18 9:57:20 CST		
Date Processed:	2017-7-18 10:43:48 CST		

Auto-Scaled Chromatogram

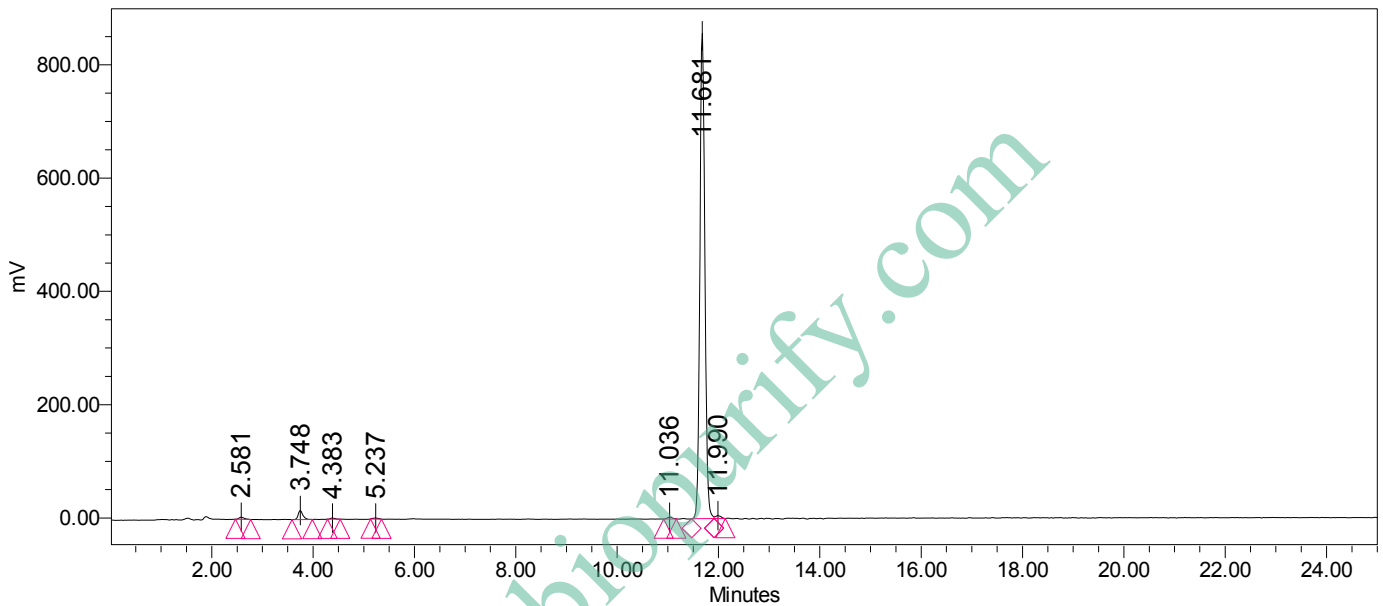

Peak Results

	Name	RT	Area	% Area	USP Plate Count	USP Resolution
1		2.581	26457	0.43	3276.9	
2		3.748	105464	1.72	7960.0	6.7
3		4.383	11532	0.19	11769.4	3.8
4		5.237	12893	0.21	6220.3	4.2
5		11.036	22019	0.36	57027.1	26.9
6		11.681	5896982	96.44	68760.8	3.4
7		11.990	39076	0.64		1.7