

产品分析证书
Certificate of Analysis

中文名称: 次乌头碱

English Name: Hypaconitine

别名 (Alias): Deoxymesaconitine; Japaconitine B1;
Japaconitine C; Japaconitine C1

产品编码 (Cat. No.): BP0750


CAS Number: 6900-87-4

分子式 (M. F.): C₃₃H₄₅NO₁₀

分子量 (M. W.): 615.72

批号 (Batch No.): PRF8022841

报告日期 (Report date): 2017年2月28日

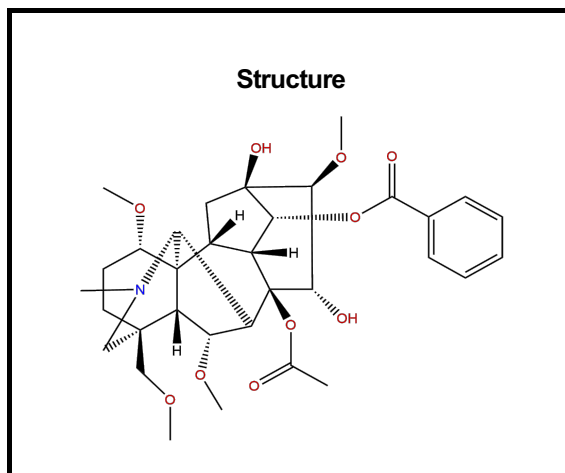

检验结果 (Analytical result):

检验项目 (Test Item)	检验指标 (Specifications)	检验结果 (Results)
外观 Appearance	Off-white solid	Off-white solid
干燥失重 Loss on drying	<3.0%	0.79%
纯度 Purity (HPLC-DAD, 235nm)*	≥98.0%	98.45%
质谱 Mass	615.72±1	Conforms
核磁 NMR	Comply with the structure	Conforms

* 色谱图见附件 (Please find HPLC chromatography attached.)

检测方法 (Test method) Column : Agilent 5 HC-C18, 4.6*250mm, 5.0um; Column temperatur : 30; Flow Rate : 1.0ml/min; Detection

Mode : UV235nm; Sample dissolution : Methanol ; Mobile Phase : A, Triethylamine- Phosphoric acid in Water (PH=7) B , Acetonitrile ;

Isocratic elution : B, 56%.

贮存条件 (Storage) : 2~8℃, protected from light, keep package airproofed when not in use.

复测期 (Retest date) : two years (2019-02-27) under conditions list above.

QC:

Zhang Ling

Date: 2017年2月28日



QA:

Wu Qi

Date: 2017年2月28日

备注 (Remarks): The sample solutions should be prepared and used on the same day, it is the best preparing the solutions immediately before use. If the solutions have to be made up in advance, it should be made as aliquots in tightly sealed vials at less than -20℃. Generally, these might be useable for up to two weeks.

In case of quality issue, please contact us within 15 days after receipt of the product.


Tel: +86-28-82633397 Fax: +86-28-82633165

http://www.phytopurify.com Email: sales@biopurify.com biopurify@gmail.com

SAMPLE INFORMATION

Sample Name:	Hypaconitine	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	
Vial:	13	Acq. Method Set:	Hypaconitine
Injection #:	1	Processing Method:	Samples
Injection Volume:	10.00 ul	Channel Name:	235.0nm
Run Time:	20.0 Minutes	Proc. Chnl. Descr.:	PDA 235.0 nm
Date Acquired:	2017-2-28 14:17:10 CST		
Date Processed:	2017-2-28 15:10:21 CST		

Auto-Scaled Chromatogram

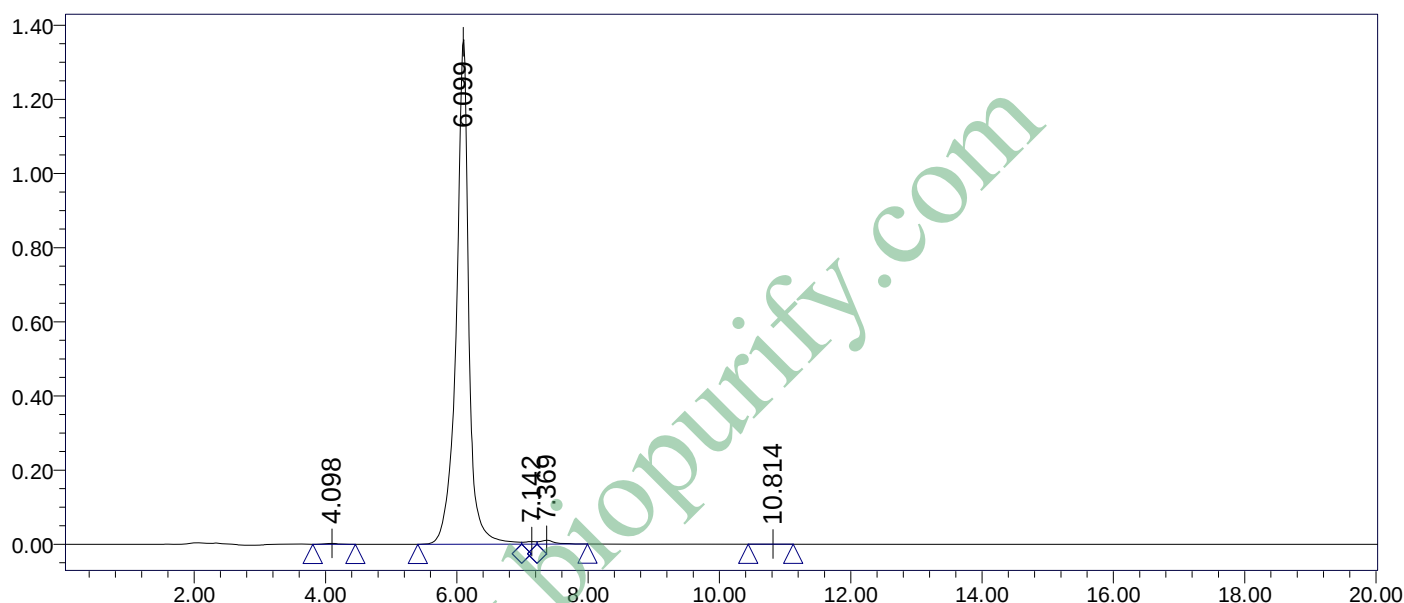

Peak Results

	RT	Area	% Area	USP Plate Count	USP Resolution
1	4.098	28889	0.16	2228.02	
2	6.099	17995663	98.45	6456.73	5.95
3	7.142	84011	0.46		
4	7.369	156942	0.86		
5	10.814	14031	0.08	4925.40	