

产品分析证书

Certificate of Analysis

中文名称：异黄腐醇

English Name : Isoxanthohumol

别名(Alias): 4',7-Dihydroxy-5-methoxy-8-prenylflavanone; Humulol

产品编码(Cat. No.):BP0805


CAS Number: 70872-29-6

分子式(M. F.): C₂₁H₂₂O₅

分子量(M. W.): 354.402

批号(Batch No.): PRF8102743

报告日期(Report date): 2017-10-27

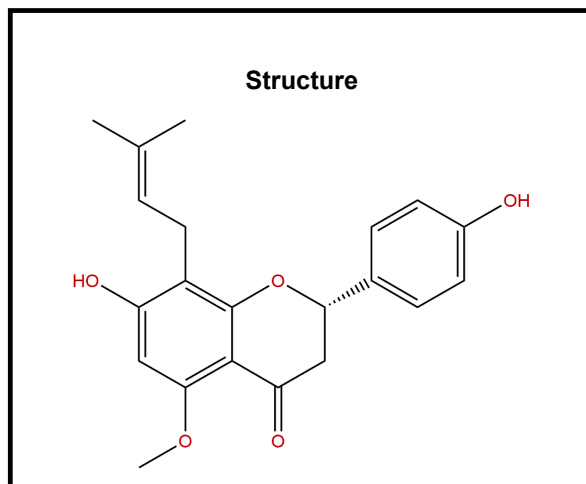

检验结果 (Analytical result) :

检验项目 (Test Item)	检验指标 (Specifications)	检验结果 (Results)
外观Appearance	Off-white cotton-like solid	Off-white cotton-like solid
干燥失重Loss on drying	< 3.0%	1.8%
纯度Purity (HPLC-DAD,290nm)*	≥98.0%	98.40%
质谱Mass	354.4±1	Conforms
核磁NMR	Comply with the structure	Conforms

* 色谱图见附件 (Please find HPLC chromatography attached.)

检测方法 (Test Method) : Column: Thermo HyPURITY C18 , 4.6*150mm , 3.0um; Column temperature: 30°C; Detection Mode: UV290nm; Flow Rate: 1.0ml/min; Sample dissolution: Methanol; Mobile Phase: A,0.1% phosphoric acid in water B, Acetonitrile ; Gradient elution: B, 30%-50%, 15min.

贮存条件 (Storage) : 2~8°C, protected from light, keep package airproofed when not in use.

复测期 (Retest date) : two years (2019-10-26) under conditions list above.

QC: Zhang Ling

Date: 2017-10-27

QA: Wu Qi

Date: 2017-10-27

备注(Remarks): The sample solutions should be prepared on the same day, it is the best preparing the solutions immediately before use. If the solutions have to be made up in advance, it should be made as aliquots in tightly sealed vials at less than -20°C. Generally, these might be useable for up to two weeks.

In case of quality issue, please contact us within 15 days after receipt of the product.




Tel: +86-28-82633397 Fax: +86-28-82633165

http://www.phytopurify.com Email: sales@biopurify.com biopurify@gmail.com

SAMPLE INFORMATION

Sample Name: Isoxanthohumol	Acquired By: System
Sample Type: Unknown	Sample Set Name:
Vial: 111	Acq. Method Set: Isoxanthohumol
Injection #: 1	Processing Method: Samples
Injection Volume: 10.00 ul	Channel Name: 290.0nm
Run Time: 25.0 Minutes	Proc. Chnl. Descr.: PDA 290.0 nm
Date Acquired: 2017-10-27 13:25:18 CST	
Date Processed: 2017-10-27 13:53:34 CST	

Auto-Scaled Chromatogram

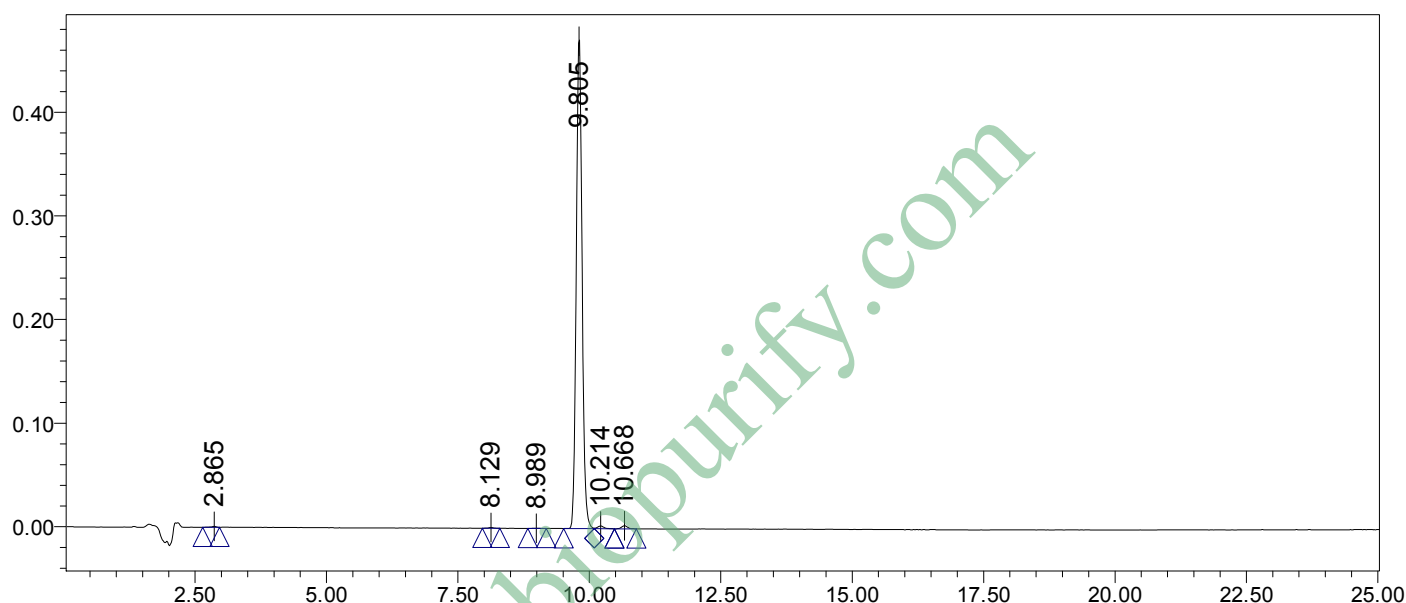

Peak Results

	RT	Area	% Area	USP Plate Count	USP Resolution
1	2.865	5735	0.16	5912.93	
2	8.129	5517	0.15	28065.52	28.92
3	8.989	1927	0.05	29554.36	4.28
4	9.805	3621500	98.40	38852.92	4.04
5	10.214	22820	0.62	35577.44	1.92
6	10.668	22766	0.62	42741.59	2.10