

产品分析证书
Certificate of Analysis

中文名称: 佛手柑素

English Name: Bergamottin

别名 (Alias): Bergaptol geranyl ether; 5-Geranyloxypsoralen; Bergaptin

产品编码 (Cat. No.): BP0255


CAS Number: 7380-40-7

分子式 (M. F.): C₂₁H₂₂O₄

分子量 (M. W.): 338.403

批号 (Batch No.): PRF8071822

报告日期 (Report date): 2017-07-18

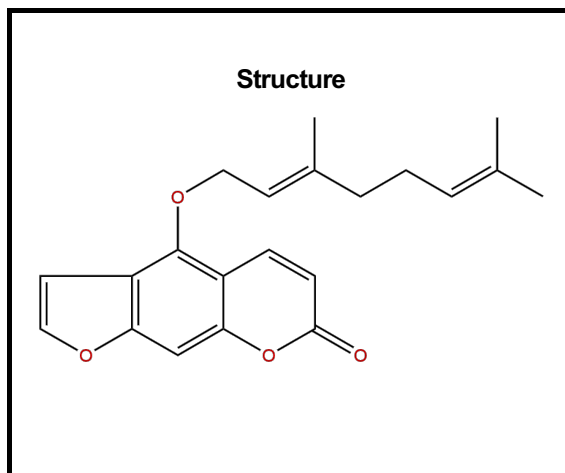

检验结果 (Analytical result):

检验项目 (Test Item)	检验指标 (Specifications)	检验结果 (Results)
外观 Appearance	Off-white needle-like crystals	Off-white needle-like crystals
干燥失重 Loss on drying	<3.0%	1.73%
纯度 Purity (HPLC-DAD, 250nm)*	≥98.0%	99.21%
质谱 Mass	338.4±1	Conforms
核磁 NMR	Comply with the structure	Conforms

* 色谱图见附件 (Please find HPLC chromatography attached.)

检测方法 (Test Method): Column: Thermo HyPURITY C18, 4.6*150mm, 3.0μm; Column temperature: 30°C; Detection Mode: UV250nm;

Flow Rate: 1.0ml/min; Sample dissolution: Methanol; Mobile Phase: A: 0.1% phosphoric acid in water B: Acetonitrile; Gradient elution: B, 65%-80%, 20min.

贮存条件 (Storage): 2-8°C, protected from light, keep package airproofed when not in use.

复测期 (Retest date): two years (2019-07-17) under conditions list above.

QC: Zhang Ling

Date: 2017-07-18

QA: Wu Qi

Date: 2017-07-18

备注 (Remarks): The sample solutions should be prepared and used on the day of receipt. It is the best preparing the solutions immediately before use. If the solutions have to be made up in advance, it should be made as aliquots in tightly sealed vials at less than -20°C. Generally, these might be useable for up to two weeks.

In case of quality issue, please contact us within 15 days after receipt of the product.


Tel: +86-28-82633397 Fax: +86-28-82633165

http://www.phytopurify.com Email: sales@biopurify.com biopurify@gmail.com

SAMPLE INFORMATION

Sample Name:	Bergamotone PRF8071822	Acquired By:	System
Sample Type:	Standard	Sample Set Name:	
Vial:	118	Acq. Method Set:	Bergamotone
Injection #:	1	Processing Method:	Samples
Injection Volume:	10.00 ul	Channel Name:	250.0nm
Run Time:	25.0 Minutes	Proc. Chnl. Descr.:	PDA 250.0 nm
Date Acquired:	2017-7-18 16:24:32 CST		
Date Processed:	2017-7-18 17:00:46 CST		

Auto-Scaled Chromatogram

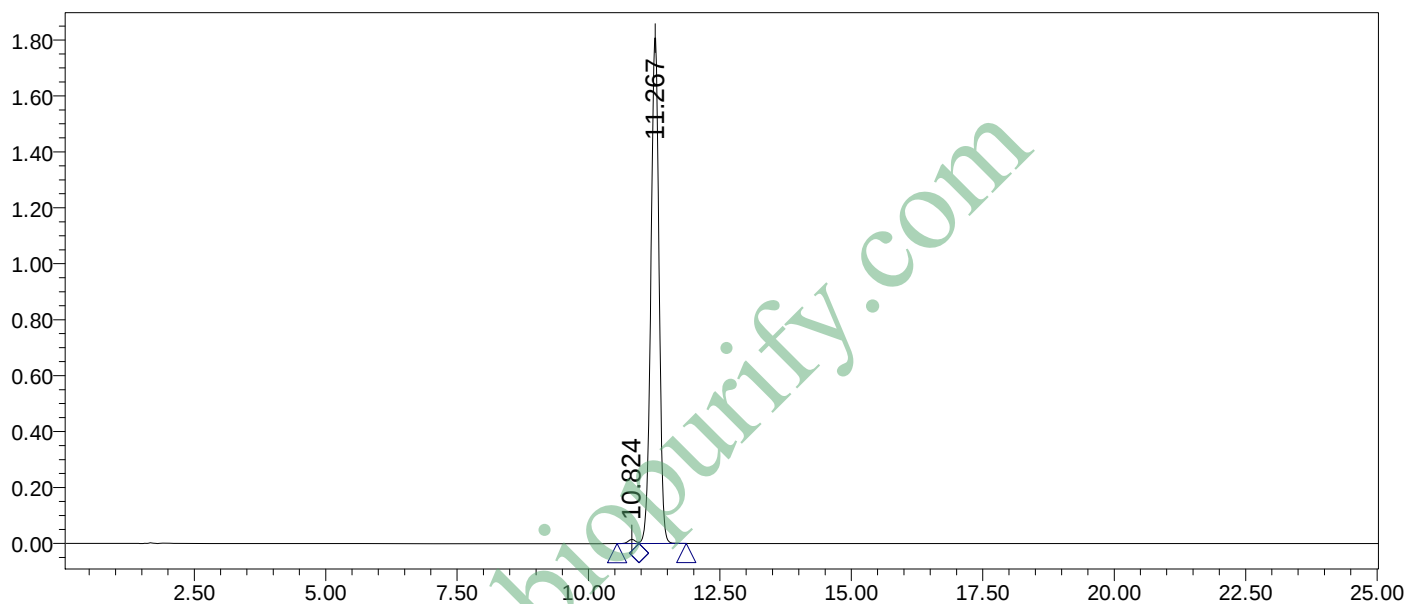

Peak Results

	RT	Area	% Area	USP Plate Count	USP Resolution
1	10.824	154921	0.79	23070.74	
2	11.267	19440406	99.21	25779.67	1.52