

产品分析证书
Certificate of Analysis

中文名称: 丁内未利葡萄糖苷

English Name: Tinnevellin glucoside

别名 (Alias):

产品编码 (Cat. No.): BP1627


CAS Number: 80358-06-1

分子式 (M. F.): C₂₀H₂₄O₉

分子量 (M. W.): 408.403

批号 (Batch No.): PRF8062841

报告日期 (Report date): 2017-06-28

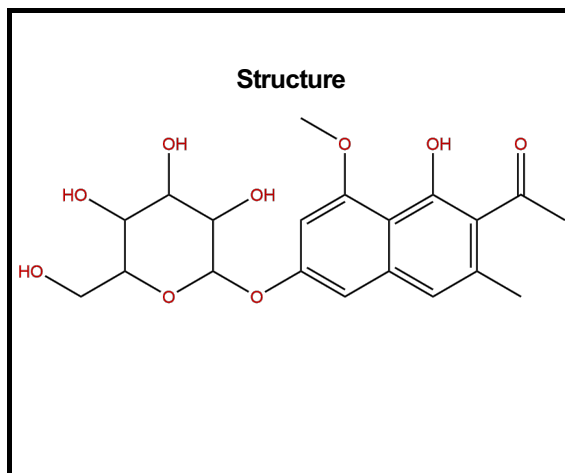

检验结果 (Analytical result):

检验项目 (Test Item)	检验指标 (Specifications)	检验结果 (Results)
外观 Appearance	Khaki powder	Khaki powder
干燥失重 Loss on drying	<3.0%	1.65%
纯度 Purity (HPLC-DAD, 230nm)*	≥98.0%	98.84%
质谱 Mass	408.4±1	Conforms
核磁 NMR	Comply with the structure	Conforms

* 色谱图见附件 (Please find HPLC chromatography attached.)

检测方法 (Test Method): Column: Thermo HYPURITY C18, 4.6*150mm, 3.0um; Column temperature: 30°C; Detection Mode: UV230nm;

Flow Rate: 1.0ml/min; Sample dissolution: Methanol; Mobile Phase: A, 0.1% phosphoric acid in water B, Acetonitrile; Gradient elution: B, 20%-25%, 20min.

贮存条件 (Storage): 2~8°C, protected from light, keep package airproofed when not in use.

复测期 (Retest date): two years (2019-06-27) under conditions list above.

QC: Zhang Ling

Date: 2017-06-28

QA: Wu Qi

Date: 2017-06-28

备注 (Remarks): The sample solutions should be prepared and used on the same day. It is the best preparing the solutions immediately before use. If the solutions have to be made up in advance, it should be made as aliquots in tightly sealed vials at less than -20°C. Generally, these might be useable for up to two weeks.

In case of quality issue, please contact us within 15 days after receipt of the product.


Tel: +86-28-82633397 Fax: +86-28-82633165

http://www.phytopurify.com Email: sales@biopurify.com biopurify@gmail.com

SAMPLE INFORMATION

Sample Name:	Tinnevellin glucoside	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	
Vial:	43	Acq. Method Set:	Tinnevellin glucoside
Injection #:	1	Processing Method:	Samples
Injection Volume:	10.00 ul	Channel Name:	230.0nm
Run Time:	25.0 Minutes	Proc. Chnl. Descr.:	PDA 230.0 nm
Date Acquired:	2017-6-28 10:12:51 CST		
Date Processed:	2017-6-28 12:54:10 CST		

Auto-Scaled Chromatogram

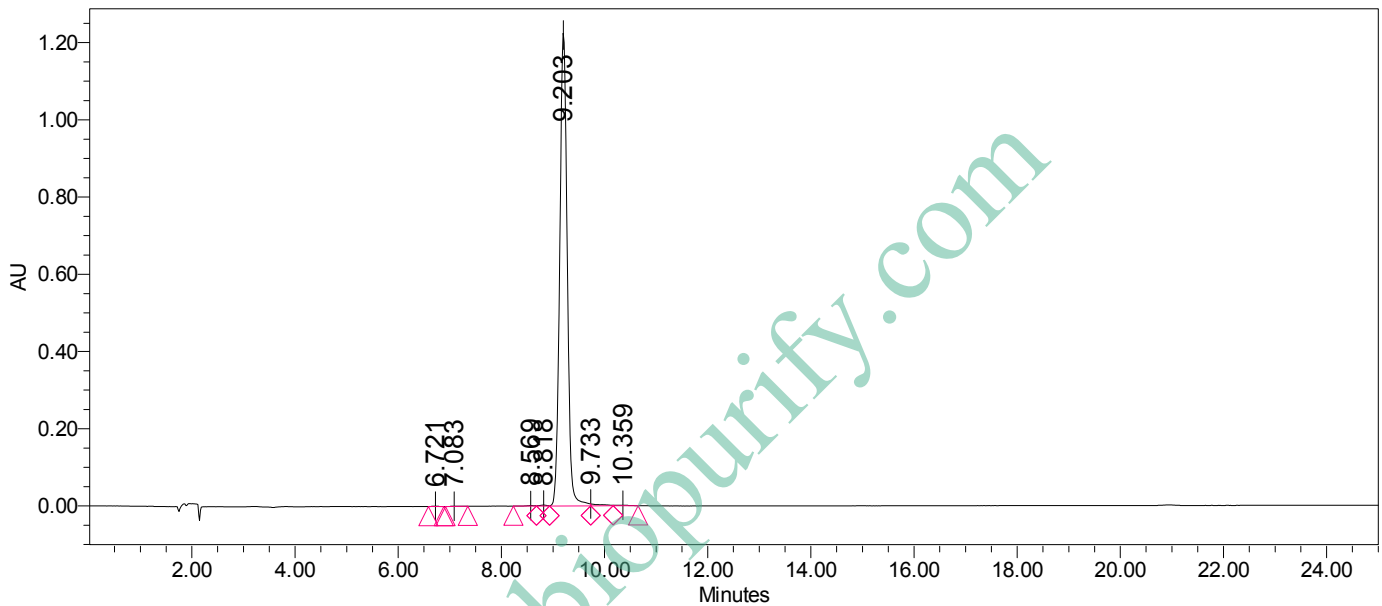

Peak Results

	Name	RT	Area	% Area	USP Plate Count	USP Resolution
1		6.721	6695	0.05	15932.8	
2		7.083	5721	0.05	16949.0	1.3
3		8.569	16418	0.13	7557.1	4.5
4		8.818	22155	0.18	13830.5	0.8
5		9.203	12313050	98.84	19889.0	1.4
6		9.733	72277	0.58		2.0
7		10.359	21738	0.17		