产品分析证书
Certificate of Analysis


中文名称：罗汉果苷 IIIe

English Name：Mogroside IIIe
别名(Alias):

产品编码(Cat. No.):BP1555
CAS Number: 88901-37-5
分子式(M. F.): C48H82O19
分子量(M. W.): 963.165

批号(Batch No.): PRF8030702
报告日期(Report date): 2017年3月7日

Structure

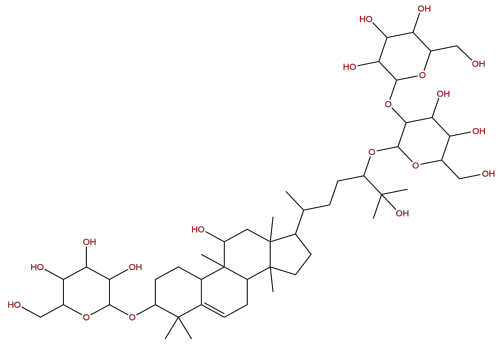

检验结果（Analytical result）：

检验项目（Test Item）	检验指标（Specifications）	检验结果（Results）
外观Appearance	Off-white powder	Off-white powder
纯度Purity (HPLC-DAD, 215nm)*	≥98.0%	98.46%
质谱Mass	963.165±1	Conforms
核磁NMR	Comply with the structure	Conforms
水分Water Content	＜3.0%	1.83%

* 色谱图见附件（**Please find HPLC chromatography attached.**）

检测方法（Test Method）： **Column**: Thermo BDS HYPERSIL C18, 4.6*100mm，2.4um; **Column temperature**: 30℃; **Detection Mode**: 215nm; **Flow Rate**: 1.0ml/min; **Sample dissolution**: Methanol ; **Mobile Phase: A**, Water, **B**, Acetonitrile; **Gradient elution:** B, 15%-35%,15min.

贮存条件（**Storage**）:2~8℃, protected from light, keep package airproofed when not in use.

复测期（**Retest date**）:two years (2019-03-06) under conditions list above.

QC: Zhang Ling
Date: 2017年3月7日

QA: Wu Qi
Date: 2017年3月7日

备注(Remarks): The sample solutions should be prepared and used promptly. It is the best preparing the solutions immediately before use. If the solutons have to be made up in advance, it should be made as aliquots in tightly sealed vials at less than -20℃. Generally, these might be useable for up to two weeks.
In case of quality issue, please contact us within 15 days after receipt of the product.


Chengdu Biopurify Phytochemicals Ltd. 质检专用章 Quality Approval Seal

Tel：+86-28-82633397 Fax：+86-28-82633165
http://www.phytopurify.com Email：sales@biopurify.com biopurify@gmail.com

SAMPLE INFORMATION

Sample Name:	Mogroside IIIe PRF8030702	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	
Vial:	18	Acq. Method Set:	Mogroside IIIe
Injection #:	1	Processing Method:	Samples
Injection Volume:	10.00 ul	Channel Name:	215.0nm
Run Time:	25.0 Minutes	Proc. Chnl. Descr.:	PDA 215.0 nm
Date Acquired:	2017-3-7 13:26:49 CST		
Date Processed:	2017-3-7 16:28:33 CST		

Auto-Scaled Chromatogram

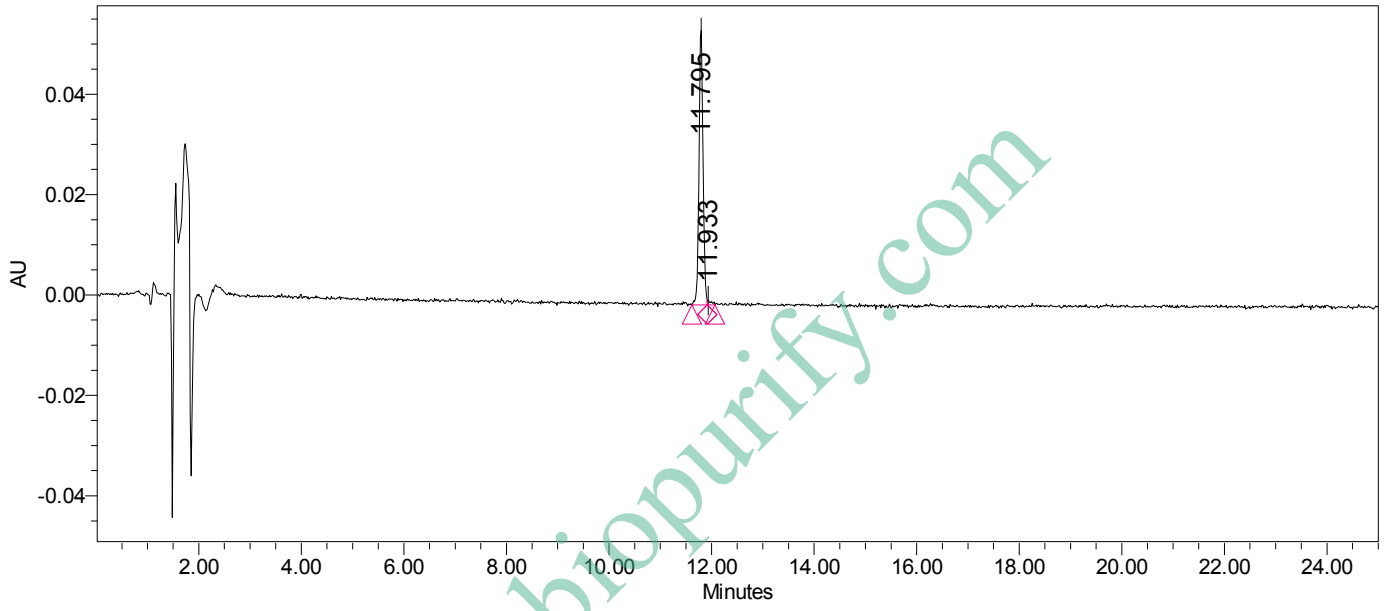

www.biopurify.com

Peak Results

	Name	RT	Area	% Area	USP Plate Count	USP Resolution
1		11.795	296556	98.46	112460.5	
2		11.933	4640	1.54		0.9